



Universiteit
Leiden
The Netherlands

Flow-based arterial spin labeling: from brain to body

Franklin, S.L.

Citation

Franklin, S. L. (2022, June 16). *Flow-based arterial spin labeling: from brain to body*. Retrieved from <https://hdl.handle.net/1887/3309826>

Version: Publisher's Version

License: [Licence agreement concerning inclusion of doctoral thesis in the Institutional Repository of the University of Leiden](#)

Downloaded from: <https://hdl.handle.net/1887/3309826>

Note: To cite this publication please use the final published version (if applicable).

Chapter 2

Influence of the cardiac cycle on velocity selective and acceleration selective arterial spin labeling.

S.L. Franklin, S. Schmid, C. Bos, M.J.P. van Osch.

¹C.J. Gorter Center for High Field MRI, Department of Radiology,
Leiden University Medical Center, Leiden, The Netherlands

²Center for Image Sciences, University Medical Centre Utrecht, Utrecht, The Netherlands

³Leiden Institute for Brain and Cognition, Leiden University, Leiden, The Netherlands

ABSTRACT

Purpose: In this study, the influence of the cardiac cycle on the amount of label produced by a velocity-selective (VSASL) and acceleration-selective arterial spin labeling (AccASL) module was investigated.

Methods: A short-PLD sequence was developed where a single VSASL- or AccASL-module was preceded by pCASL labeling to isolate the arterial blood pool. ASL subtraction was performed with label/control images with similar cardiac phase and time-of-measurement, followed by retrospective binning in ten cardiac phase bins. ASL signal variation over the heart cycle was evaluated and tested for significance using a permutation test.

Results: VSASL and AccASL showed significant arterial signal fluctuations over the cardiac cycle of up to respectively ~36% and ~64%, mainly in areas containing large arteries. pCASL also showed significant signal fluctuations, of up to ~25% in arteries. Raw label/control images confirmed that the observed signal fluctuations were caused by the amount of label produced during the cardiac cycle, rather than inflow-effects, since the raw images did not all show equal cardiac phase dependence.

No significant effects of the cardiac cycle were found on the gray matter ASL-signal.

Conclusion: Significant influence of the cardiac cycle on the generated label was found for spatially non-selective ASL-sequences. Hence, in order to become independent of the cardiac cycle, sufficient averages need to be taken. Alternatively, these findings could be highly interesting for the purpose of quantifying pulsatility more distally in the vascular tree.

INTRODUCTION

Arterial Spin Labeling (ASL) is a non-invasive MRI technique allowing quantitative perfusion measurements by magnetically labeling arterial blood. In traditional ASL, blood proximal to the imaging volume is magnetically altered in the label image, followed by a post-labeling-delay (PLD) where the labeled blood flows into the imaging region. By subtracting this label image from a control image in which the inflowing magnetization is unaltered, static tissue signal is removed and only perfusion signal is left.

However, in traditional ASL transit delay artefacts can arise when not all of the labeled blood has reached the imaging volume during the PLD, thereby leading to underestimation of the perfusion and occurrence of vascular artefacts. In velocity-selective (VSASL) and acceleration-selective ASL (AccASL) blood is not labeled based on location, but based on flow velocity and acceleration, respectively. This implies that labeling is also performed within the imaging volume, thereby reducing tissue transit-delay artifacts[49]. The VSASL-module creates label by saturating spins above a certain cut-off velocity[49], or in case of Fourier-transform based velocity selective inversion (FT-VSI), inverting spins below the cut-off velocity[53]. The AccASL-module creates label by saturating spins above a certain cut-off acceleration/deceleration[51]. By labeling closer to the target region, VSASL and AccASL offer not only advantages in patients with slow-flow, but also in functional MRI (fMRI) experiments where ASL is used as readout[79], [80].

However, since velocity and acceleration of blood varies over the cardiac cycle, it is our hypothesis that the amount of label generated will depend on the cardiac phase in which the VSASL- or AccASL-module is applied. Previously, the cardiac cycle has already been shown to influence signal stability in other ASL techniques, such as pulsed-ASL[81], [82] and pCASL[83]. Inflow of fresh blood[83] as well as transit time[81], [82] have been mentioned as mechanisms through which the cardiac cycle influences signal stability. In case of VSASL and AccASL it is important to know whether the cardiac cycle has a significant effect on the amount of label that is generated to allow correct quantification and interpretation of these techniques, as well as to maximize temporal SNR, which can be considered especially important for functional applications[79]. In the current study the effect of the cardiac cycle on the amount of label that is produced is examined by using only a *single* VSASL(AccASL)-module with a short PLD, in combination with pCASL pre-pulse to limit the saturation-effect of the VSASL- and AccASL-modules to *arterial* blood, thereby avoiding contamination by venous signal.

In summary, the aim of this study is to investigate whether the amount of label generated by a VSASL- or AccASL-module depends on the cardiac phase during which the labeling takes place.

METHODS

General approach

Both VSASL- and AccASL-modules consist of motion sensitizing gradients, which are switched-on in label condition and switched-off in control condition. The VSASL gradients have alternating polarity, creating label by saturating spins above a certain cut-off velocity, whereas the AccASL gradients all have a positive polarity resulting in saturation above an acceleration threshold. Subtracting label from control thus generates signal from the saturated spins, i.e. the spins above the cut-off velocity(acceleration).

The original VSASL-sequence consists of two VSASL-modules with the same cut-off velocity: the first module is either in label or control condition, whereas the second module is played out after a PLD of 1-2 seconds and is always in label (velocity crushing) condition. The purpose of the second module is to provide a well-defined end to the bolus, enabling quantification, and to remove the venous component of the VSASL signal. The original AccASL implementation consists of only a single AccASL-module, since it inherently has very limited venous labeling[51].

To study the influence of the cardiac cycle it is important to be able to control the timing of labeling with respect to the cardiac cycle. This means that the effects of a *single* VSASL(AccASL)-module on the arterial blood pool need to be isolated. However, using only a single VSASL-module would result in a mixture of arterial and venous signal and, since arterial and venous systems overlap at tissue level, it would be very hard to isolate the labeled arterial blood using an arterial or venous mask. Therefore, a pCASL-preparation was used to first isolate the arterial signal, which was subsequently saturated by the spatial non-selective single VSASL(AccASL)-module, see Figure 1. Before adopting this experimental design, we also employed the same approach in a prospectively triggered fashion, see Supporting Information Figure S1. The prospectively triggered sequence had a very long pCASL-labeling duration (>7s), to become insensitive to differences in labeling duration. However, results of this approach were inconclusive, see Supporting Information Figure S2 and S3. Details of the methods and results of this experiment are reported in the Supporting Information.

Combining pCASL and a single VSASL- or a AccASL-module in one sequence yields four control/label conditions, since both the pCASL- and VSASL(AccASL)-module can be in label or control condition, see Figure 1B. Our main parameters of interest are VSArt and AccArt, see Figure 1C, which represent the amount of pCASL label, i.e. arterial blood, that is saturated by the VSASL- or AccASL-module. VSArt and AccArt are calculated by subtracting the pCASL image with VSASL- or AccASL-crushing from a regular pCASL image. Other possible subtractions and their interpretations, are described in Figure 1C. Whereas our analysis focuses on

VSArt and AccArt-images as a function of cardiac phase, single-VSASL(AccASL) images will also be shown to allow evaluation of the effectiveness of the pCASL pre-pulse to isolate the arterial blood pool, nevertheless it should be noted that the single-VSASL(AccASL)-image will partially contain venous signal. In addition, the pCASL images will be shown to provide information on cardiac phase dependence of label generation by pCASL.

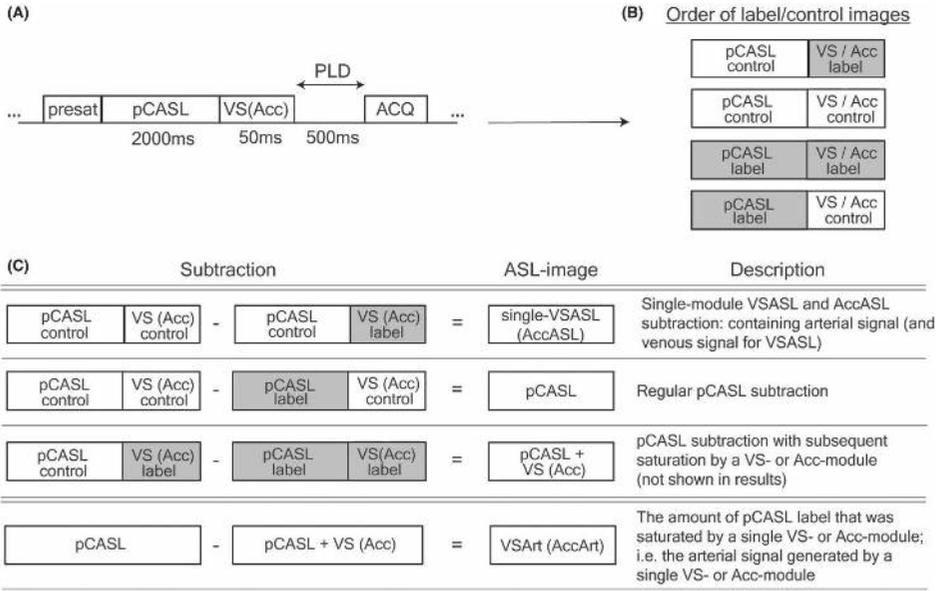


Figure 1 A) Sequence diagram for the scans combining pCASL and a VSASL- or AccASL-module. B) Order of label/control conditions for four consecutive acquisitions, this was repeated 200 times. C) Subtractions of the label/control images and their descriptions.

In-vivo experiments

In total fourteen healthy volunteers were scanned, seven (22–56 years, 3 men and 4 women) with pCASL-VSASL, and seven (19–59 years, 3 men and 4 women) with pCASL-AccASL. All volunteers were screened for MRI contra-indications, and provided written informed consent. Cardiac phase was recorded continuously using a peripheral pulse unit (PPU) on the finger of the volunteer. A PPU-triggered phase-contrast quantitative flow scan, planned on the internal carotid arteries (at the location of the pCASL labeling), was acquired in order to measure blood flow velocity as a function of cardiac phase and to be able to measure the delay in occurrence of the R-peak as measured by PPU and maximum velocity at labeling location. For post-processing a 3D T_1 -weighted scan was acquired to obtain a gray matter mask, and a whole-brain phase-contrast angiography (PCA) scan was acquired to allow the generation of an arterial mask.

MRI acquisition parameters

Scans were acquired on a Philips 3T MRI scanner (Ingenia CX, Philips, Best, The Netherlands) using a multi-slice single-shot EPI readout and a 32-channel head coil.

The ASL scans were acquired with a TR/TE of 3204ms/16ms, and 200 repetitions per label/control condition, resulting in a total scan time of 43 minutes. Presaturation of the imaging region was employed before pCASL-labeling using a WET-pulse[84]. The labeling duration of pCASL was set to 2000ms, which is longer than the average tissue arrival time[85] to make sure that pCASL-signal filled the whole arterial side of the vasculature and to minimize any influence of the cardiac cycle on the distance that label will travel into the (micro)vasculature. The VSASL cut-off velocity was set to 1.9cm/s and the AccASL cut-off acceleration to 1.3m/s². Background suppression pulses were applied during pCASL labeling at 50 and 1150ms. See Table 1 for all scan parameters. A relatively short PLD of 500ms was chosen to reduce cardiac phase dependent effects on the transport of label, i.e. transit delay, as well as cardiac phase dependent inflow from ‘fresh’ spins which did not experience presaturation, while still ensuring enough time for VSASL(AccASL)-gradient induced eddy currents to decay.

Parameter	ASL scans	
Voxel size	3x3x7mm ³	
Number of slices	17	
TR	3204ms	
TE	16ms	
Number of repetitions	200 (per label/control condition)	
Background suppression pulses	50/1150ms	
Total scan time	43 minutes	
Post-labeling delay	500ms	
pCASL labeling duration	2000ms	
	VSASL	AccASL
Labeling module duration	50ms	50ms
Gradient duration	0.8ms	0.8ms
Gradient strength	17mT/m	30mT/m
Cut-off velocity/acceleration	1.9cm/s	1.3m/s ²

Table 1. Scan parameters for the retrospectively triggered ASL scans.

The phase-contrast quantitative flow measurement was PPU-triggered and acquired using a single slice 2D-FFE readout, with a TR/TE of 13/8.0ms, retrospectively reconstructed in 15 heart-phases, with voxels sizes of 0.6/0.6/6mm, and a phase-contrast encoding velocity of 200cm/s, resulting in a total scan duration of 2 min 57 s. In addition, a whole-brain PCA scan was acquired using a 3D-FFE readout, with a TR/TE of 20/4.0ms, reconstructed voxel sizes of 1.1/1.1/1.75mm, and a phase-contrast encoding velocity of 30cm/s, resulting in a total scan

duration of 53 s. The 3D-T₁w scan was acquired using a multi-shot 3D-TFE readout, with a TR/TE of 9.7/4.6ms, using reconstructed voxel sizes of 0.9/0.9/1.2mm, resulting in a total scan duration of 4 min 57 s.

Postprocessing

ASL images were realigned (SPM 12, University College London, London, United Kingdom) and data analysis was conducted using MATLAB R2015b (The MathWorks, Inc., Natick, MA, United States of America). In regular ASL, label and control images are acquired in an interleaved fashion to prevent subtraction errors arising from scanner drift. In the current study not only scanner drift but also cardiac phase needed to be taken into account. Since the four label/control images were not triggered on cardiac phase, no predefined, sequentially acquired label-control pairs with the same cardiac phase were available for subtraction. Thus, images with similar times of measurement as well as cardiac phase needed to be found to perform the subtractions. Suitable images for subtraction were created by performing Gaussian-weighted averaging within the “time-of-measurement/cardiac phase”-plane, see Figure 2. A Gaussian kernel was moved over the plane with a step size of $\pi/5$ in cardiac phase direction and $36 \cdot TR$ in time-of-measurement direction, to obtain a grid of 22×10 data points for each label/control condition. The Gaussian kernel was designed such that it had a full-width-half-maximum of a step size, leading to blurring of half a step size in both directions; 18° (i.e. $\pi/10$) in cardiac phase direction and $18 \cdot TR = 58$ seconds in time-of-measurement direction. Subtractions between the label/control conditions were performed per grid point, and then averaged per cardiac phase bin.

Arterial and gray matter masks were generated to be able to obtain separate gray matter- and arterial signal curves. To this end, the pCASL image was co-registered separately to the T₁-based gray matter segmentation and the whole-brain PCA scan. The inverse transformation matrix was consequently applied to respectively the T₁-based gray matter segmentation and PCA scan, which were then both reformatted to the same space and resolution as the ASL images (all performed in SPM12). A vascular mask was generated by thresholding of the whole-brain PCA scan. Next, an arterial mask was generated by selecting only those voxels in the vascular mask that had an intensity above a manually-determined threshold on the mean pCASL image. A gray matter mask was generated by segmenting the 3D T₁-weighted scan (SPM12). Lastly, voxels from the gray matter segmentation that were also part of the vascular mask were removed. The arterial and gray matter mask were used to generate separate arterial and gray matter signal intensity curves of all ASL images as a function of cardiac phase.

The phase-contrast quantitative flow scan provided blood flow velocity curves over the cardiac cycle relative to the moment of PPU-trigger detection, allowing temporal alignment of label generation to the cardiac cycle and corresponding blood flow velocities. From the PPU-

triggered phase-contrast quantitative flow scan, the delay in occurrence of the R-peak measured by the PPU and maximum velocity at the pCASL-labeling location, was calculated. The R-peak delay was used to correct the cardiac phase of the blood flow velocity curves as well as the ASL data points, which were then plotted on a scale of zero to 2π to become independent of the heart rate interval.

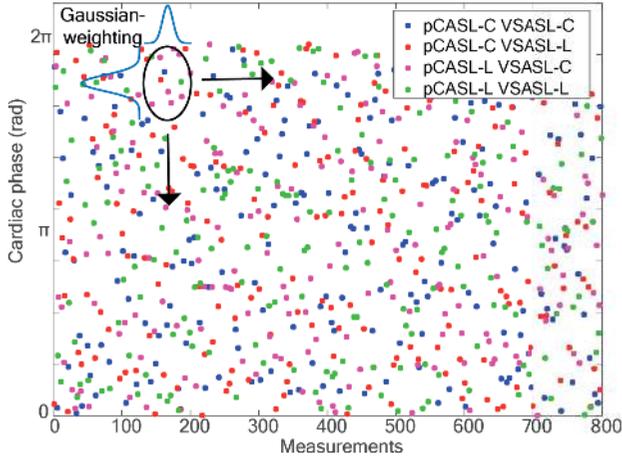


Figure 2. Averaging of the raw label/control images for the retrospectively triggered scans to obtain suitable subtraction of images with similar time-of-measurement and cardiac phase, to prevent subtraction errors from scanner drift and cardiac phase differences. Graph shows all the data points acquired in a single scan session. Four different raw images were acquired: pCASL_{control}, pCASL_{label}, followed by either VSASL_{control} or VSASL_{label}. The plot shows how a Gaussian-weighted average was taken of each of the four label/control conditions, and within the ellipse, which was moved over the “measurement time-cardiac phase” plane in 22 steps in time-of-measurement direction, and 10 in cardiac phase direction, to obtain a grid of 22×10 data points for each label/control condition. Subtractions of the label/control conditions were performed per grid-point. Lastly, the data was averaged per cardiac phase bin.

To test whether the signal intensity fluctuations of the ASL images over the cardiac cycle were significantly larger than could be expected from the noise-level, a permutation test was performed where the cardiac phases were randomly reassigned to other data points before the Gaussian-weighted averaging step in the data analysis pipeline. Using the same permutations for all volunteers, the variance of the resulting signal intensity curves over the cardiac cycle ($\text{Var}_{v,p}^{\text{norm},\text{random}}$) was calculated per permutation p and volunteer v and compared to the variance of the non-permuted data ($\text{Var}_v^{\text{norm},\text{card}}$). In total 600 permutations were performed. Subject-specific $\text{Var}_{v,p}^{\text{random}}$ values were normalized according to their average $\overline{\text{Var}_v^{\text{random}}}$ over the 600 permutations allowing to pool data from all volunteers, resulting in a normalized $\text{Var}_{v,p}^{\text{norm},\text{random}}$. Next, a distribution was built by calculating the mean normalized variance over all volunteers per permutation $\overline{\text{Var}_p^{\text{norm},\text{random}}}$, representing the normalized variances that can be expected when data points are not sorted based on their correct cardiac phase. Based on this distribution, the percentile belonging to the actual measured mean normalized variance $\overline{\text{Var}_p^{\text{norm},\text{card}}}$ over all volunteers (i.e. using the correct cardiac phase) was calculated. The measured fluctuations were deemed to be significant if the percentile was $>95\%$ (α of 0.05).

Analogous to Li et al⁸ we examined the phase dependence of the raw label/control images to be able to rule out that the fluctuations in signal are simply caused by inflow of “fresh” spins that have not experienced presaturation. Should the fluctuations be caused by inflow of fresh spins, then the raw images would exhibit the same dependence on cardiac phase, since all will be affected similarly by fresh inflow, whereas difference in label generation would not affect all raw images in the same way.

RESULTS

Figure 3 shows the perfusion-weighted images for: VSArt, single-VSASL, and pCASL at ten cardiac phase bins for a representative volunteer. Figure 4 shows the perfusion-weighted images for AccArt, single-AccArt and pCASL for a representative volunteer. The zoomed-in part shows that VSArt, AccArt, single-AccASL and pCASL have minimal signal in the superior sagittal sinus, the main draining vein of the brain, while single-VSASL does show some signal there. The difference between VSArt and single-VSASL indicates the expected venous labeling for single-VSASL, and shows that isolation of arterial signal in VSArt by use of pCASL as a pre-pulse was effective, see Figure 3. To focus on the signal variation over the cardiac cycle, the mean image over all cardiac phases was subtracted from the images, see Figure 5 and 6. The signal especially fluctuates in areas containing large arteries, which is supported by the signal intensity curves in Figure 7.

Results from the permutation test showed that the arterial signal variance over the cardiac cycle was significantly higher than expected by chance in most ASL images, (VSArt $P = 0.017$, AccArt $P = 0.010$, single-AccASL $P = 0.047$, pCASL (VS dataset) $P = 0.015$ and pCASL (Acc dataset) $P = 0.024$). Within the group of volunteers in which velocity-selective labeling was applied, a signal change up to $\sim 36\%$ was found for VSArt, and $\sim 26\%$ for pCASL in the arteries. Single-VSASL did not show significant signal fluctuations over the cardiac cycle ($P = 0.202$), although a trend similar to the fluctuations of VSArt can be observed in Figure 7.

For the acceleration-selective experiments similar results were observed, with a signal change up to $\sim 64\%$ for AccArt, 29% for single-AccASL and $\sim 24\%$ for pCASL in arteries. Comparing the signal fluctuations with the blood flow velocity and acceleration shows that the blood flow velocity peak seems to coincide with the signal intensity peak of VSArt and pCASL, while the AccArt and single-AccASL peak is more similar to the peak in blood flow acceleration. The signal variance over the cardiac cycle in gray matter was not significantly increased.

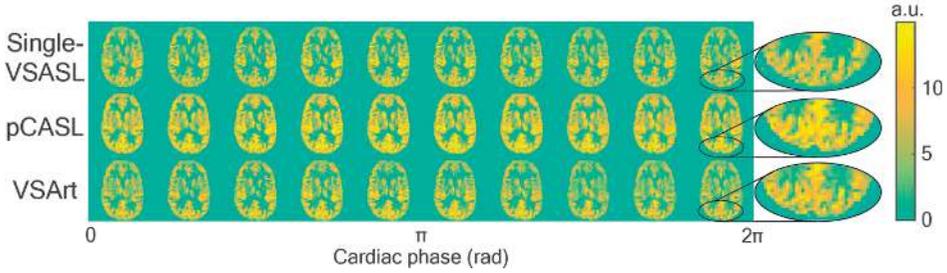


Figure 3. Perfusion-weighted images over the cardiac cycle of a representative volunteer for VSASL. The first row represents single-VSASL, the second row pCASL, the third row represents VSArt, i.e. the single-VSASL confined to the arterial blood pool as obtained by subtracting pCASL+VS (not shown) from regular pCASL (row 2). A zoom-in of the ellipse is shown to highlight the presence of venous signal in the sagittal sinus for single-VSASL, in contrast to pCASL, VSArt, single-AccASL, and AccArt.

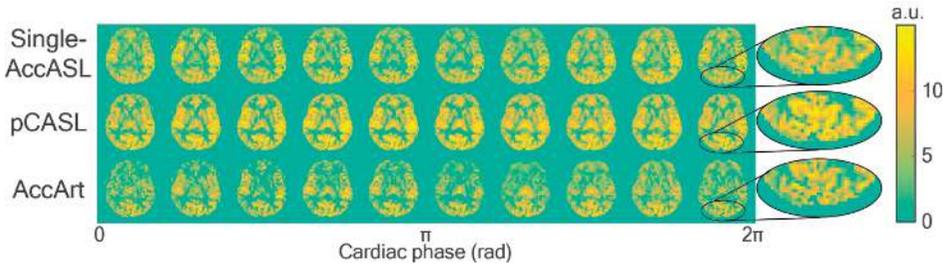


Figure 4. Perfusion-weighted images over the cardiac cycle of a representative volunteer for AccASL. The first row represents single-AccASL, the second row pCASL, the third row represents AccArt, i.e. the single-AccASL confined to the arterial blood pool as obtained by subtracting pCASL+Acc (not shown) from regular pCASL (row 2). A zoom-in of the ellipse is shown to highlight the absence of venous signal in the sagittal sinus for single-AccASL, pCASL, and AccArt, in contrast to single-VSASL.

Figure 8 shows the intensity curves of the raw label/control images before subtraction. Averaged over all volunteers, a pattern emerges, if the pCASL- and VSASL-module are both in either label or control condition, $[pCASL_{\text{control}} VSASL(AccASL)_{\text{control}}]$ and $[pCASL_{\text{label}} VSASL(AccASL)_{\text{label}}]$ the signal shows less fluctuations than if either one of them is in label condition and the other in control, $[pCASL_{\text{label}} VSASL(AccASL)_{\text{control}}]$ and $[pCASL_{\text{control}} VSASL(AccASL)_{\text{label}}]$, this is most prominently found for AccASL.

DISCUSSION & CONCLUSIONS

VSASL and AccASL are two promising ASL-techniques with reduced transit-time artefacts, where labeling is done based on respectively spin velocity and acceleration as opposed to location as done in traditional ASL. The fact that labeling is performed based upon velocity and acceleration raises the question whether the amount of label that is generated will vary over the cardiac cycle. In this study, the effect of the cardiac cycle on label generation by a *single* VSASL- and AccASL-module was investigated.

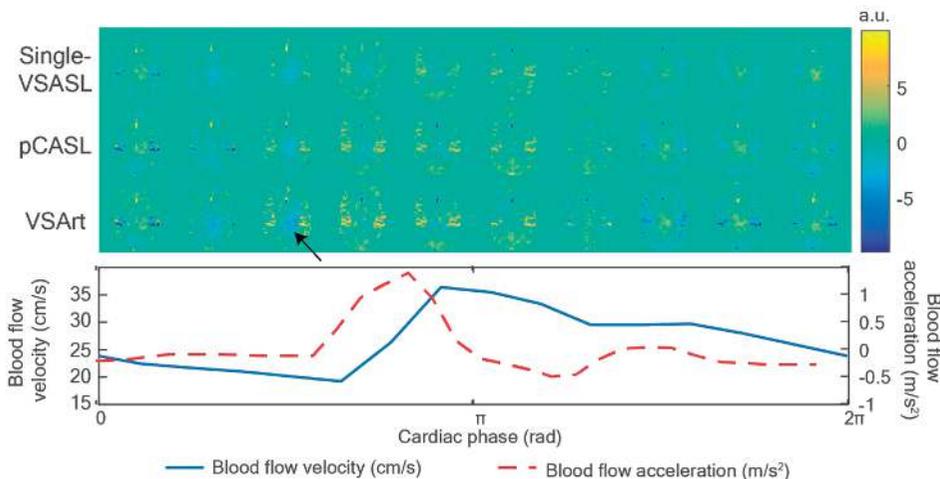


Figure 5. Perfusion-weighted images with the mean over the cardiac cycle subtracted for a representative volunteer for VSASL, showing the variation over the cardiac cycle with respect to the mean. Below, the corresponding blood flow velocity and acceleration are shown over the cardiac phases. Note that in these images negative signal means that the signal is below the average over the whole cardiac cycle. The first row represents single-VSASL, the second row pCASL, the third row represents VSArt, i.e. the single-VSASL confined to the arterial blood pool as obtained by subtracting pCASL+VS (not shown) from regular pCASL (row 2). Arrows indicate cardiac-dependent signal fluctuations in an area unrelated to perfusion, this signal is believed to stem from sub-optimal background suppression, see discussion. Bottom: corresponding blood flow velocity measurement in the carotid artery, as a function of cardiac phase.

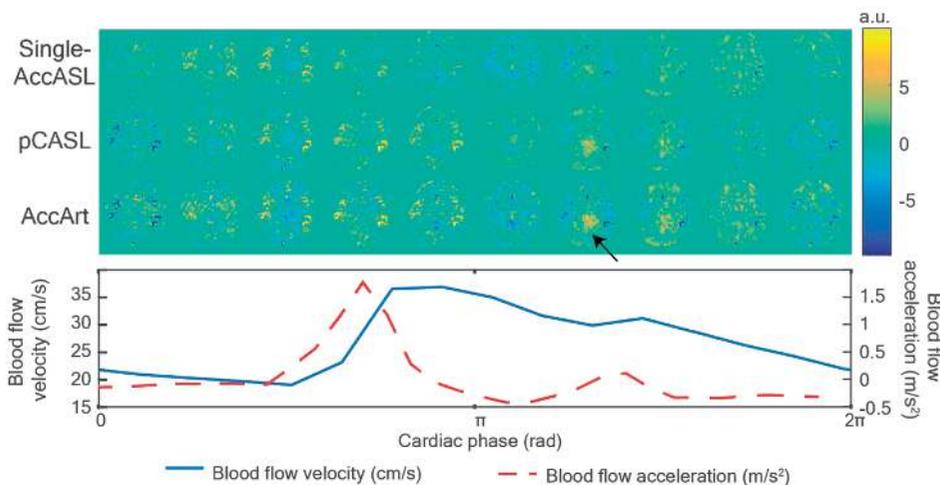


Figure 6. Perfusion-weighted images with the mean over the cardiac cycle subtracted for a representative volunteer for AccASL, showing the variation over the cardiac cycle with respect to the mean. Below, the corresponding blood flow velocity and acceleration are shown over the cardiac phases. Note that in these images negative signal means that the signal is below the average over the whole cardiac cycle. The first row represents single-AccASL, the second row pCASL, the third row represents AccArt, i.e. the single-AccASL confined to the arterial blood pool as obtained by subtracting pCASL+Acc (not shown) from regular pCASL (row 2). Arrows indicate cardiac-dependent signal fluctuations in an area unrelated to perfusion, this signal is believed to stem from sub-optimal background suppression, see discussion. Bottom: corresponding blood flow velocity measurement in the carotid artery, as a function of cardiac phase.

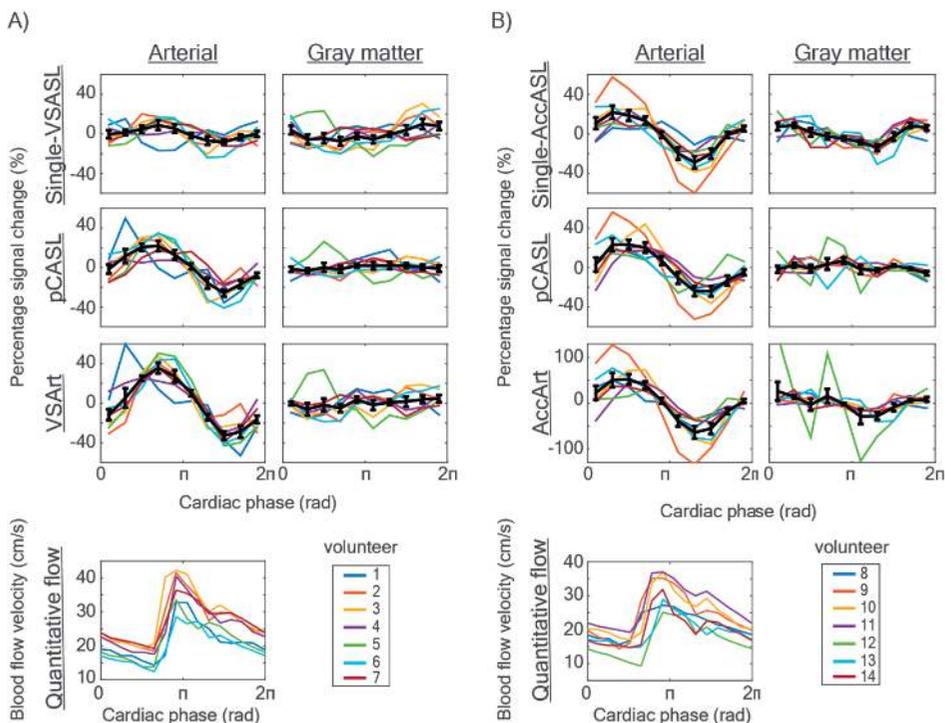


Figure 7. Signal intensity curves for A) VSASL and B) AccASL, over the ten cardiac phase bins. Left column: using arterial mask, right column: using gray matter mask. From top to bottom; the first row represents single-VSASL(AccASL), the second row pCASL, the third row represents VSArt(AccArt), i.e. the single-VSASL(AccASL) confined to the arterial blood pool as obtained by subtracting pCASL+VS(Acc) (not shown) from regular pCASL (row 2). All results are aligned according to the volunteer-specific blood velocity peak in the quantitative flow measurement, shown in the last row. Results are shown for all seven volunteers in each group. The black line in each graph represents the mean signal over the volunteers, with error bars indicating the standard error of the mean. Note that the y-axis scale of AccArt deviates from the rest. Volunteer 12 from the AccASL-dataset showed deviating signal fluctuations in the gray matter; however, exclusion of this volunteer from the analyses, neither affected statistical findings nor changed our conclusions.

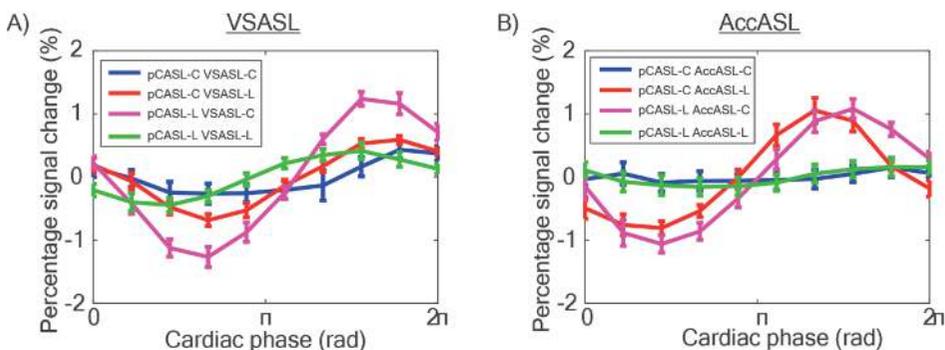


Figure 8. Arterial signal intensity plots of the four label/control images before subtraction; [pCASL_{control} VSASL_{control}], [pCASL_{control} VSASL_{label}], [pCASL_{label} VSASL_{control}] and [pCASL_{label} VSASL_{label}], of A) VSASL dataset and B) AccASL dataset. Mean intensity averaged over all volunteers is plotted, including error bars indicating the standard error of the mean. The label/control conditions are not all influenced equally by the cardiac cycle. Cardiac cycle fluctuation is less for the conditions with both pCASL and VSASL in label or control state ([pCASL_{control} VSASL_{control}] and [pCASL_{label} VSASL_{label}]), as compared to the conditions where either one of the two ASL-methods is in control state ([pCASL_{label} VSASL_{control}] and [pCASL_{control} VSASL_{label}]).

A sequence was designed to minimize cardiac-dependent effects on the signal by 1) inflow, 2) distance that the label travels into the vasculature, and 3) venous signal. Specifically, a single VSASL- or AccASL-module was combined with a pCASL preparation to limit its effect to the arterial blood pool. A short PLD was used to limit fresh inflow, and the pCASL-labeling duration was chosen longer than the average tissue transit time[85] to exclude influence of variations in the distance that label will travel into the microvasculature. Arterial label should intentionally be isolated for single VSASL(AccASL)-labeling since it also results in venous labeling, which in a regular VSASL sequence with two labeling modules is filtered out by the second labeling module. ASL images were retrospectively binned based on the cardiac phase during which labeling took place. Results confirm the hypothesis that VSASL(AccASL)-labeling of the arterial blood pool (VSASL/AccASL) depends on the cardiac cycle, where the AccASL signal showed higher signal fluctuations (up to 64%) than VSASL (up to 36%). In addition, pCASL (up to 25%), and single-AccASL (up to 29%) showed significant signal fluctuations over the cardiac cycle.

Effectiveness of the pCASL pre-pulse to isolate arterial signal is confirmed by the obtained VSASL and single-VSASL images. Single-VSASL, in contrast to VSASL, showed signal in the sagittal sinus, indicating the expected venous signal. Venous contributions can also explain why single-VSASL, in contrast to VSASL, did not show significant fluctuations over the cardiac cycle, since the venous signal will depend less on the cardiac cycle than the arterial part of the signal. Along the same lines, single-AccASL *did* show significant signal fluctuations since it has minimal venous labeling[51], further confirmed by the AccASL images of this study which hardly show signal in the superior sagittal sinus. However, single-AccASL still showed less signal fluctuations than AccASL, which suggests some additional signal contribution in the single-AccASL signal and possibly also in the single-VSASL signal, which is not cardiac-dependent and is filtered out using the pCASL-preparation, such as signal from diffusion-weighting caused by the VSASL- and AccASL-module[49], [51].

Results show that the peak in VSASL-signal coincides with the peak in blood flow velocity, indicating that signal fluctuations are not caused by inflow of 'fresh' spins, since then an inverse relation between ASL-signal and blood flow velocity would be expected. The observations support the hypothesis that at high blood flow velocity, more spins will flow faster than the cut-off velocity(acceleration), leading to an increase in signal. As would be expected, the AccASL-signal peak coincides more with the peak in blood flow acceleration. However, difference in timing between the peak in AccASL and VSASL-signal should be confirmed by performing VSASL and AccASL experiments in the same subjects. Finally, the peak in pCASL signal also coincided with the blood flow velocity peak; note that this timing is with respect to the end of pCASL-labeling. This means that the peak in pCASL-signal might be explained by an increase in the number of spins passing through the labeling plane (and therefore are inverted) at

end-of-labeling; moreover this effect will be enhanced due to minimal T_1 -decay for spins at end-of-labeling. However, there is also a small effect of blood flow velocity on pCASL labeling efficiency[86].

Previous studies on the effect of the cardiac cycle on ASL have mainly focused on pulsed ASL and pCASL. Our findings confirm the general finding that cardiac influence seems to be largest in regions with large arteries[82], [83], [87]–[89]. Contrary to our results, Verbree et al[90] did not observe significant fluctuations in the pCASL signal based on the cardiac phase of end-of-labeling. This was probably due to a lack of power, because of limited averaging due to very long labeling durations and the lack of background suppression, similar to our prospectively triggered approach, described in Appendix 1. Using the retrospectively triggered approach, more repetitions could be acquired, and a significant effect of the cardiac cycle on pCASL end-of-labeling was observed.

Li et al[83] observed increased pCASL signal instability for a non-triggered sequence compared to a triggered-sequence based on the cardiac phase during the readout excitation-pulse. Using a PLD of 1800ms, Li et al[83] concluded that the pCASL-signal instability was most probably caused by cardiac-dependent inflow effects instead of label generation, since both label- and control-signal showed the same phase dependence over the cardiac cycle. In the current study, an effort was made to minimize inflow effects by using a shorter PLD of 500ms, not allowing ‘fresh’ spins to enter the imaging volume. Results show that the label/control images do not all have the same phase dependence, suggesting that the fluctuations of the signal are indeed caused by differences in the amount of label generated over the cardiac cycle, rather than inflow effects. The images where pCASL and VSASL(AccASL) are not in the same condition; $[pCASL_{\text{control}} VSASL(AccASL)_{\text{label}}]$ and $[pCASL_{\text{label}} VSASL(AccASL)_{\text{control}}]$, show the highest cardiac dependence. This could be explained by the fact that label generation in both pCASL and VSASL are influenced by the cardiac cycle. A relatively high blood velocity at the start of the VSASL(AccASL) block leads to increased saturation by this module, so in case of the $[pCASL_{\text{control}} VSASL(AccASL)_{\text{label}}]$ image a relatively low signal. Similarly, for pCASL, a relatively high blood velocity at the end-of-label will lead to an increase in inverted spins at end-of-label, so a relatively low signal for $[pCASL_{\text{label}} VSASL(AccASL)_{\text{control}}]$. Images where both pCASL and VSASL(AccASL) are in control-condition show less variation, indicating that there is minimal influence from inflow of ‘fresh’ spins from outside of the field-of-view. The image where both pCASL and VSASL(AccASL) are in label-condition also shows less cardiac dependence, which could be due to a cancellation of the two labeling-methods; the cardiac phase with a relatively high blood velocity, will lead to an increase in inverted spins at pCASL end-of-labeling, however, this increased inverted magnetization could in turn be saturated by the VSASL module, since more spins will have a velocity (acceleration) above the cut-off value, essentially reducing the cardiac dependence of the signal.

Some limitations should be considered when interpreting the results. Although careful consideration was given to limit confounding factors related to the cardiac cycle which might affect the data, it is possible that cardiac variations of the pCASL-signal influenced the VSArt and AccArt measurements, potentially resulting in an overestimation in the reported cardiac dependence of the VSASL and AccASL-signal. Importantly though, since VSArt(AccArt) is a subtraction of pCASL and pCASL+VS(Acc), not all of the pCASL cardiac dependence will be propagated. Specifically, all pCASL signal below the cutoff velocity(acceleration) will be subtracted out and it is expected that a large part of the bolus will be flowing below the cutoff velocity/acceleration since the pCASL labeling duration is longer than the average tissue arrival time[85].

Another limitation of the current study is that due to the 2D-readout, later-acquired slices will effectively have a longer PLD and will not have optimal background suppression. Sub-optimal background suppression of later acquired slices have possibly resulted in the cardiac phase-dependent signal fluctuations in an area unrelated to perfusion, shown in Figure 5 and 6. The signal seems to be in anti-phase with the vascular signal and in close proximity to main CSF structures, indicated by the arrows. Both features make it likely that CSF-flow is involved in these fluctuations, but the exact origin of this signal is not completely understood. This is in accordance with a recent study which showed increased physiological noise around the ventricular system for ASL, although in that study the noise seems to be located more centrally in the brain compared to our results[91].

In addition, the interpolation step (FWHM of Gaussian kernel is 18°) as well as using a PPU-device instead of ECG for heart cycle recording will have introduced some smoothing of the data. The PPU could also have caused a small error in the cardiac phase if heart rate variability would have been high, since then the R-peak delay would have varied. However, heart rate variability during the scan session was found to be low (average standard deviation of RR interval = 0.11sec (VSASL) and 0.10sec (AccASL)), so we expect very minor effects on our conclusions considering the relatively low cardiac phase resolution of 10 cardiac phase bins. Lastly, it is likely that some partial volume effects will have been introduced by using arterial and gray matter masks during analysis (keeping in mind a slice thickness of 7mm). This will have led to some overestimation of the fluctuations in the gray matter accompanied by underestimation of fluctuations in the arteries, but these effects are expected to be relatively minor.

The finding that the amount of label generated by a VSASL(AccASL)-module fluctuates over the cardiac cycle is very interesting for understanding of the technique, the interpretation and quantification of it, and for optimizing SNR. For future studies, it would be interesting to investigate how cutoff velocity(acceleration) influences the cardiac phase dependence of the VSASL and AccASL-signal. By lowering this cut-off value, the label will be created further

into vascular tree, where pulsation might be decreased. However, investigating multiple cutoff velocities (accelerations) in the current study would have come at the cost of lower SNR and/or lower resolution over the cardiac cycle, when the total examination time would be kept constant. In addition, it would also be of interest to investigate whether VSASL or AccASL could be used to measure pulsatility in the microvasculature.

The pulse wave velocity has been known to increase with age, as well as in certain diseases, such as diabetes[92], and although the exact mechanism is still unknown, it has been associated with tissue damage in the brain[92], [93]. The current view is that the brain is very susceptible to the effects of increased pulse wave velocity because of the low vascular resistance of the brain, which exposes small capillaries to high-pressure fluctuations[92], [93]. The microvasculature will respond by increasing the resistance to limit the penetration of the pulsatility, but this may reduce blood flow and can lead to microscopic tissue damage[93]. Since microvascular disease is thought to be involved in strokes, dementia and white matter lesions[92], [93], it is thus very important to be able to measure the pulsatility in the microvasculature, something which only recently has been done in smaller penetrating arteries in a single slice using phase contrast MRI at ultra-high field[94].

In summary, this study has shown that the amount of arterial label generated by a single module of VSASL, AccASL, and pCASL can fluctuate up to respectively 36%, 64% and 25% over the cardiac cycle. By acquiring sufficient averages, this effect will be averaged out. Furthermore, the presented acquisition methodology could provide a valuable starting point for future measurement of the pulsatility at the tissue level, or at least more distally in the vascular tree than is currently possible.

ACKNOWLEDGEMENTS

This work is part of the research programme Drag ‘n Drop ASL with project number 14951, which is (partly) financed by the Netherlands Organisation for Scientific Research (NWO). S.Schmid and M.J.P. van Osch are supported by the research program Innovational

Research Incentives Scheme Vici with project number 016.160.351, which is financed by the Netherlands Organisation for Scientific Research (NWO).

SUPPORTING INFORMATION

In this paper, the influence of the cardiac cycle on the amount of label generated by VSASL and AccASL was investigated by retrospectively binning the images based on the cardiac phase at the start of the VSASL or AccASL-module. Before the retrospective method was designed a prospectively triggered method was implemented and tested, where placement of the VSASL and AccASL module with respect to the cardiac cycle was controlled using triggering. This supplementary material contains the design and results of this prospective method. Results were promising albeit inconclusive.

The methods were similar to what is described in the methods section in the main document. The main difference is that for these experiments the start of the VSASL(AccASL)-module and therefore the end of pCASL-labeling was triggered, see Supporting Information Figure S1 A. Five trigger delays were selected based on a quantitative flow phase-contrast scan performed at the pCASL-labeling location to be able to place the VSASL(AccASL)-module at five distinct cardiac phases (Supporting Information Figure S1 B). The trigger delays add an additional length to the pCASL-labeling. Since differences in labeling duration would overwhelm the effect of the cardiac cycle on VSASL(AccASL)-labeling, a very long pCASL-labeling duration of minimally 7 seconds was chosen to become independent of the extra labeling duration.


In total fifteen healthy volunteers were scanned with the prospectively triggered sequence, eight (21–35 years) with pCASL-VSASL, and seven (24–63 years) with pCASL-AccASL. In contrast to the study in the main document, considerably less averages could be acquired because of the long labeling duration of pCASL, i.e. 50 repetitions per label/control condition, resulting in a total scan time of 35 minutes. Because of the varying pCASL-labeling duration, no background suppression could be applied. Similar to the main study, a short PLD was chosen to avoid inflow of ‘fresh’ spins that did not experience pre-saturation. For the prospectively triggered study a PLD of 400ms was chosen.

Label/control images from the same cardiac phase were subtracted and averaged to obtain four ASL images, see Figure 1C in main manuscript. In contrast to the main experiments, the arterial mask was obtained by thresholding the mean pCASL-image.


From the resulting images, main arteries can be distinguished, which show variation in signal intensity over the cardiac cycle, see Supporting Information Figure S2. Supporting Information Figure S3 shows the signal intensity curves for all images. A consistent phase dependence is visible for the single-VSASL and single-AccASL images in the arterial and gray matter mask, where the signal peak corresponds to the blood flow velocity peak. Signal curves of the other ASL images (pCASL, VSArt and AccArt) show a less consistent pattern across volunteers.

Inconsistency in results is probably due to a number of reasons, of which the most important one is the fact that few repetitions could be acquired because of the long pCASL labeling duration. Secondly, no background suppression could be applied because the prospective triggering approach introduced a varying sequence length. The effect of no background suppression is especially clear in the single-AccASL images in the top panel of Supporting Information Figure S2, which show high signal in white matter and ventricles. Thirdly, images were taken at only five different cardiac phases resulting in a coarse sampling of the cardiac cycle, making it difficult to uncover the exact shape of the cardiac phase dependence of the ASL-signal. Lastly, it is possible that due to the short PLD of 400ms there is still some instability in the signal due to residual eddy currents induced by the gradients in the VSASL- or AccASL-module. The retrospective method, described in the main section of this manuscript, was implemented to overcome these issues. With the retrospective method more averages could be acquired, background suppression could be used, the cardiac cycle could be sampled in ten steps instead of five, and we used a slightly longer PLD of 500ms to reduce influence of residual eddy currents; which resulted in a more consistent pattern over the cardiac cycle.


SUPPORTING INFORMATION FIGURES

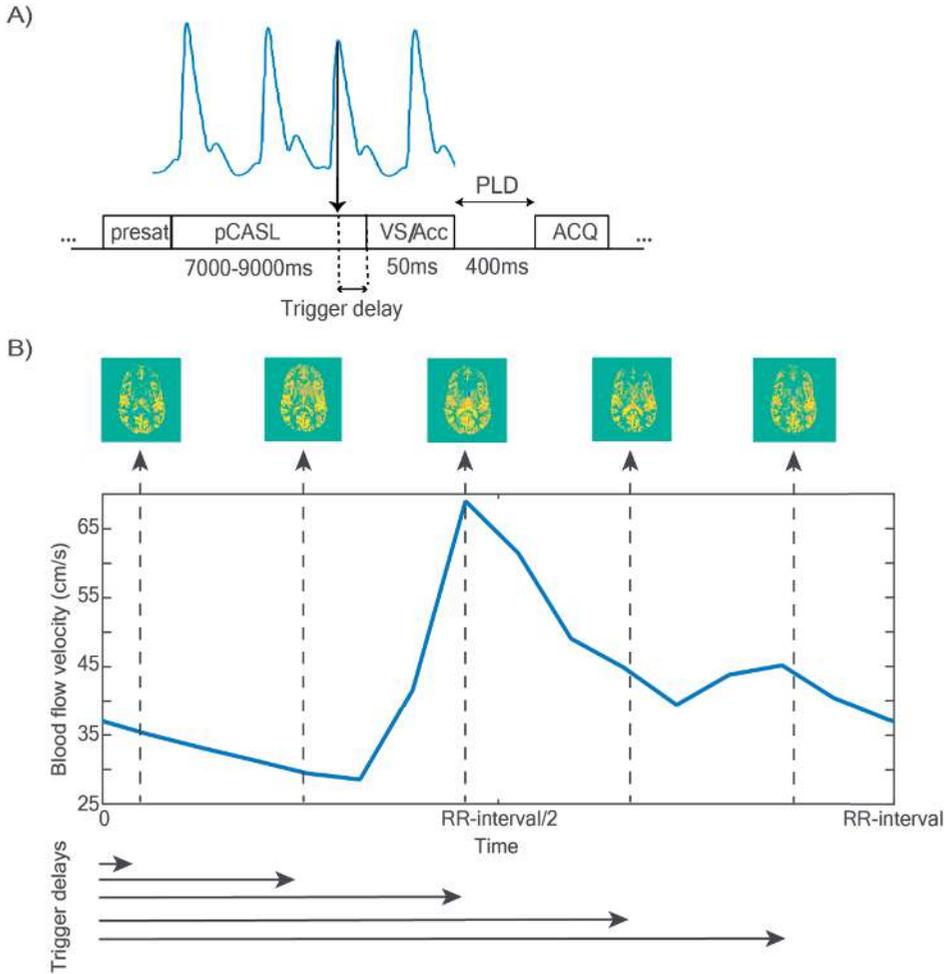

Supporting Information Figure 1. A) Sequence diagram for the prospectively triggered scans combining pCASL and a single VSASL- or AccASL-module. B) Pulse wave form as measured by a phase-contrast quantitative flow scan in the internal carotid artery at the level of the pCASL-labeling plane, used to calculate five trigger delays in the prospectively triggered scans. One trigger delay was defined on the peak of the graph, and the rest by dividing the cardiac cycle into five equal parts. Using these trigger delays, the ASL images are acquired at five different cardiac phases.

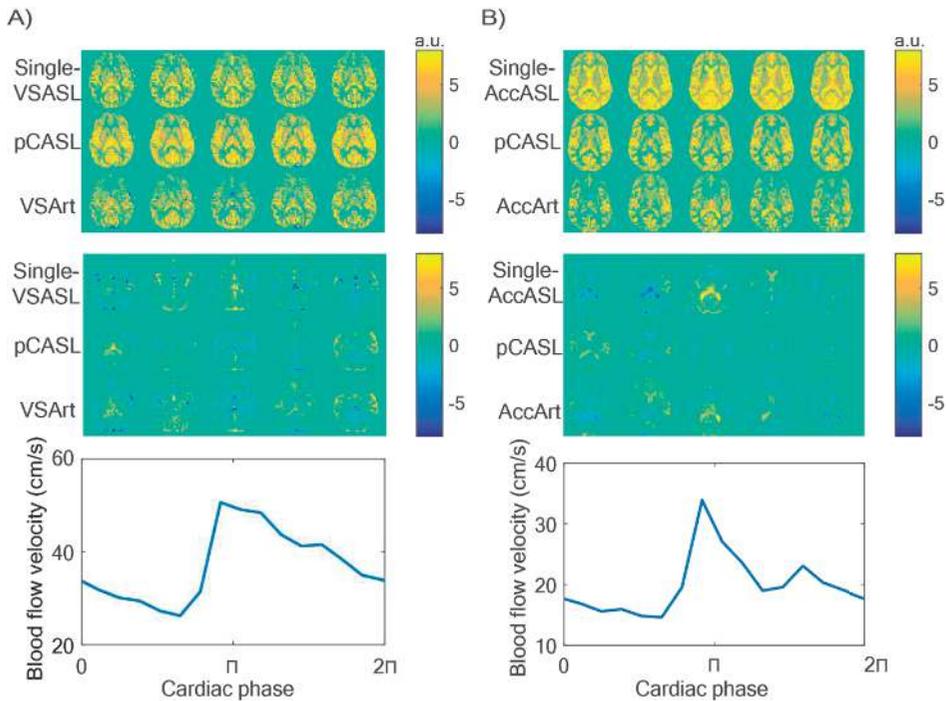

Supporting Information Figure 2. ASL images of the prospectively triggered experiments in a representative volunteer for VSASL (A) and AccASL (B), for the five cardiac phases. Top-row: original images, middle-row: images with the mean over cardiac cycle subtracted, note that a negative signal here means that the signal is below the mean signal over the whole cardiac cycle. Within each panel of images, the top row represents single-VSASL(AccASL), the second row pCASL, and the last row VSArt(AccArt); i.e. the arterial signal generated by the single VSASL(AccASL)-module as obtained by subtracting pCASL+VS(Acc) (not shown) from regular pCASL (row 2).

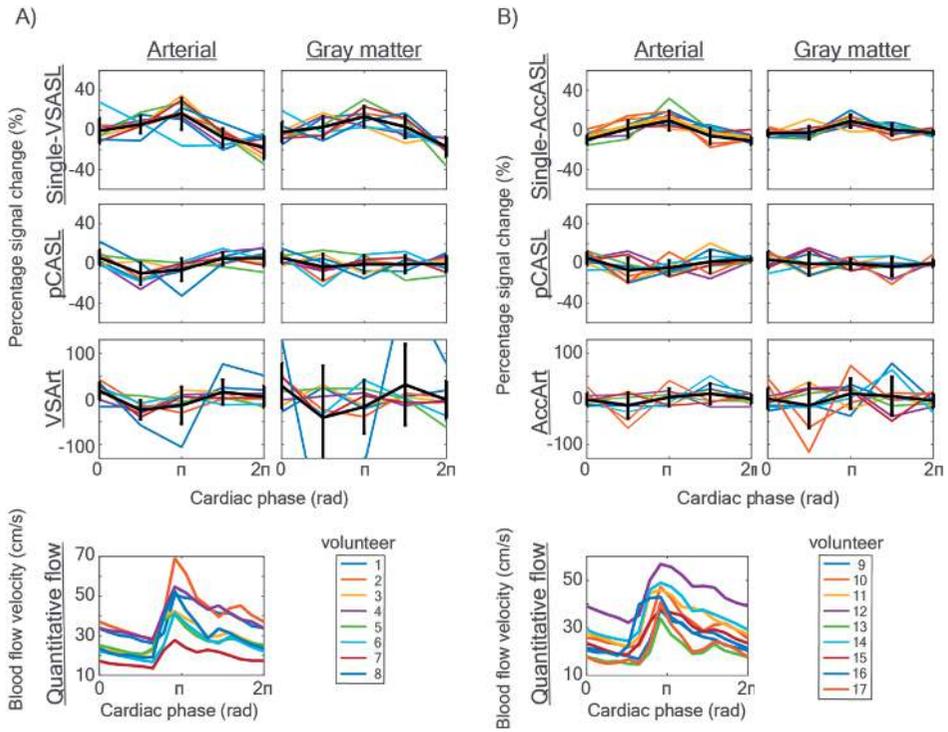

Supporting Information Figure 3. Signal intensity curves of the prospectively triggered data for A) VSASL and B) AccASL, over the five cardiac phases. Left column: arterial signal as obtained by using an arterial mask, right column: gray matter signal. From top to bottom; the first row represents single-VSASL(AccASL), the second row pCASL, the third row VSArt(AccArt); i.e. the arterial signal generated by the single VSASL(AccASL)-module as obtained by subtracting pCASL+VS(Acc) (not shown) from regular pCASL (row 2). All results are aligned according to the volunteer-specific blood velocity peak in the quantitative flow measurement, shown in the last row. Results are shown for all eight and nine volunteers in each group respectively. The black line in each graph represents the mean signal over the volunteers, with error bars indicating the standard error of the mean.

