



Universiteit
Leiden
The Netherlands

Agreement of aptamer proteomics with standard methods for measuring venous thrombosis biomarkers

Faquih, T.; Mook-Kanamori, D.O.; Rosendaal, F.R.; Baglin, T.; Dijk, K.W. van; Hylckama, A. van

Citation

Faquih, T., Mook-Kanamori, D. O., Rosendaal, F. R., Baglin, T., Dijk, K. W. van, & Hylckama, A. van. (2021). Agreement of aptamer proteomics with standard methods for measuring venous thrombosis biomarkers. *Research And Practice In Thrombosis And Haemostasis*, 5(4). doi:10.1002/rth2.12526

Version: Publisher's Version




License: [Creative Commons CC BY-NC-ND 4.0 license](#)

Downloaded from: <https://hdl.handle.net/1887/3217416>

Note: To cite this publication please use the final published version (if applicable).

BRIEF REPORT

Agreement of aptamer proteomics with standard methods for measuring venous thrombosis biomarkers

Tariq Faquih MS¹   | Dennis O. Mook-Kanamori MD, PhD^{1,2}  |
 Frits R. Rosendaal MD, PhD¹ | Trevor Baglin MD, PhD³ |
 Ko Willems van Dijk MD, PhD^{4,5,6} | Astrid van Hylckama Vlieg PhD¹

¹Department of Clinical Epidemiology, Leiden University Medical Center, Leiden, The Netherlands

²Department of Public Health and Primary Care, Leiden University Medical Center, Leiden, The Netherlands

³Medicxi Ventures LLP, London, UK

⁴Division of Endocrinology, Department of Internal Medicine, Leiden University Medical Center, Leiden, The Netherlands

⁵Eindhoven Laboratory for Experimental Vascular Medicine, Leiden University Medical Center, Leiden, The Netherlands

⁶Department of Human Genetics, Leiden University Medical Center, Leiden, The Netherlands

Correspondence

Tariq Faquih, Department of Clinical Epidemiology, Leiden University Medical Center, Postal Zone C7-P, PO Box 9600, 2300 RC, Leiden, The Netherlands.
 Email: t.o.faquih@lumc.nl

Funding information

This project was sponsored by the Leiden University Fund/Nypels van der Zee fonds. THE-VTE study was supported by the Netherlands Organization for Scientific Research, grant number 916.56.157 (VENI)]. Tariq Faquih was supported by the King Abdullah Scholarship Program and King Faisal Specialist Hospital & Research Centre (No. 1012879283).

Handling Editor: Dr Neil Zakai.

Abstract

Background: Venous thromboembolism (VTE) is a complex disease with an incidence rate of about 1 in 1000 per year. Despite the availability of validated biomarkers for VTE, unprovoked events account for 50% of first events. Therefore, emerging high-throughput proteomics are promising methods for the expansion of VTE biomarkers. One such promising high-throughput platform is SomaScan, which uses a large library of synthetic oligonucleotide ligands known as aptamers to measure thousands of proteins.

Objective: The aim of this study was to evaluate the viability of the aptamer-based SomaScan platform for VTE studies by examining its agreement with standard laboratory methods.

Methods: We examined the agreement between eight established VTE biomarkers measured by SomaScan and standard laboratory immunoassay and viscosity-based instruments in 54 individuals (27 cases and 27 controls) from the Thrombophilia, Hypercoagulability and Environmental Risks in Venous Thromboembolism study. We performed the agreement analysis by using a regression model and predicting the estimates and the 95% prediction interval (PI) of the laboratory instrument values using SomaScan values.

Results: SomaScan measurements exhibited overall poor agreement, particularly for D-dimer (average fit, 492.7 ng/mL; 95% PI, 110.0-1998.2) and fibrinogen (average fit, 3.3 g/L; 95% PI, 2.0-4.7).

Conclusion: Our results indicate that SomaScan measurement had poor agreement with the standard laboratory measurements. These results may explain why some genome-wide association studies with VTE proteins measured by SomaScan did not confirm previously identified loci. Therefore, SomaScan should be considered with caution in VTE studies.

KEYWORDS

aptamers, biomarkers, blood coagulation factors, immunoassay, nucleotide, proteomics, venous thrombosis

This is an open access article under the terms of the Creative Commons Attribution-NonCommercial-NoDerivs License, which permits use and distribution in any medium, provided the original work is properly cited, the use is non-commercial and no modifications or adaptations are made.

© 2021 The Authors. *Research and Practice in Thrombosis and Haemostasis* published by Wiley Periodicals LLC on behalf of International Society on Thrombosis and Haemostasis (ISTH).

Essentials

- Measurement agreement of aptamer proteomics for venous thromboembolism (VTE) markers is unknown.
- We selected 27 cases with unprovoked VTE and 27 controls from the Thrombophilia, Hypercoagulability and Environmental Risks in Venous Thromboembolism study.
- Agreement between the aptamers and the laboratory methods for the VTE biomarkers was poor.
- Currently, the usage of aptamer proteomics for VTE biomarkers should be considered with caution.

1 | INTRODUCTION

Venous thromboembolism (VTE) is a complex disease caused by an imbalance in the coagulation and fibrinolysis pathways. VTE, which encompasses deep vein thrombosis (DVT) and pulmonary embolism (PE), has an incidence rate of 1 in 1000 per year.¹ VTE is assumed to be caused by both acquired and genetic risk factors,¹ but the mechanisms that evoke VTE involve complex interactions of pathways that are still not fully understood.^{1,2} Several genetic variants and proteins and have been identified as risk factors for VTE, such as factor V Leiden (*F5 rs6025*), prothrombin 20210A (*FII rs1799963*), low levels of antithrombin, protein S and protein C, and high levels of factors VIII, IX, and XI.¹

The current standard methods to quantify coagulation factors are by viscosity or optical detection-based coagulation analyzers and immunoassay-based laboratory instruments targeting one or more coagulation factors. For example, elevated levels of D-dimer are associated with increased risk of DVT, recurrent DVT, and mortality.³ Moreover, D-dimer is measured with >95% diagnostic sensitivity by immunoassay-based instruments and hence broadly used by clinicians for the exclusion of VTE in patients with low or intermediate risk.⁴

Further expansion of the number of biomarkers is imperative for studying the etiology and improving prediction of VTE. Emerging high-throughput proteomic platforms are promising tools to identify such novel biomarkers, as these platforms are capable of quantifying large numbers of proteins simultaneously from a single sample.^{5,6} The aim of our study was to assess the measurement agreement of one such platform, the aptamer-based SomaScan platform, by comparing its measurements with the current established laboratory methods for eight VTE biomarkers in the Thrombophilia, Hypercoagulability and Environmental Risks in Venous Thromboembolism (THE-VTE) study.

1.1 | SomaScan

SomaScan (SomaLogic, Inc, Boulder, CO, USA) is a high-throughput proteomics platform capable of simultaneous measurement of thousands of proteins. Unlike traditional immunoassay instruments, SomaScan uses systematic evolution of ligands by exponential enrichment, a biochemical technique used to create a library with a wide range of modified synthetic oligonucleotide ligands (known as aptamers) designed to bind to their respective protein targets. Aptamers provide several benefits over immunoassay methods:

They are inexpensive to produce, highly modifiable, and chemically stable. SomaScan has developed a vast library of unique aptamers to detect thousands of proteins.⁷ This makes the SomaScan platform appealing for researchers, and, indeed, several large studies have used the platform for various purposes including the identification of novel protein markers.⁸⁻¹⁰

2 | METHODS

2.1 | THE-VTE study

For our cases and controls, we used samples from the THE-VTE study, a multicenter case-control study from Leiden, The Netherlands, and Cambridge, United Kingdom.¹¹ Inclusion took place between March 2003 and December 2008. In total, 626 patients were included, aged 18 to 75, with a first DVT or PE. Partners of the patients were invited as controls. Subsequent follow-up of the cases was performed to assess recurrence risk. The mean follow-up duration was 4.8 years after discontinuation of oral anticoagulant therapy. Blood samples were taken 2 to 3 months after discontinuation of anticoagulants. The blood samples were collected into Sarstedt Monovette tubes, in a 0.1 volume of 0.106 M trisodium citrate and separated into plasma by centrifugation then stored at -80°C . All participants gave written informed consent. The study was approved by the Medical Ethics Committee of the Leiden University Medical Centre in Leiden, The Netherlands, and the NHS Research Ethics Committee in Cambridge, United Kingdom.

The current pilot study was originally designed to explore the biomarker measurement differences between unprovoked VTE and controls in a case-control design using SomaScan. Before proceeding, we checked the general measurement agreement between SomaScan and standard laboratory immunoassay and viscosity-based instruments in both cases and controls to assess the agreement over the whole range of coagulation factor levels. Unprovoked events were defined as individuals who did not have surgery, trauma, or long-term immobilization 3 months before the event. Moreover, patients were excluded if they had an active malignancy; abnormal levels of proteins C, protein S, and antithrombin (<80 U/dL); or used hormone replacement therapy or hormonal contraceptives at the time of the event. Patients with factor V Leiden or prothrombin (PT20210A) mutations were also excluded. We selected a sample of 16 cases with unprovoked VTE and further added 11 patients who experienced a recurrent venous thrombosis during follow-up, resulting in the inclusion of 27 VTE cases. By including unprovoked

VTE cases as well as controls, we covered a wide range of VTE biomarker values. Finally, we randomly selected 27 participants without VTE as controls. The frozen samples of the selected cases and controls were sent and thawed for analysis by SomaScan in 2016. No thawing or refreezing was performed during the interim period between 2011 and 2016. VTE biomarkers were measured by validated immunoassay-based, viscosity-based detection instruments, henceforth referred to as laboratory instruments. D-dimer total concentration (nanograms per milliliter) was measured by the Vidas D-dimer immunoassay (BioMérieux, Marcy-l'Etoile, France). The activity (international units per milliliter) of protein C, protein S, antithrombin (using chromogenic assay), prothrombin, coagulation factor IX, and coagulation factor XI were measured by a STA-R coagulation analyzer (Diagnostica Stago, Parsippany, NJ, USA). Fibrinogen total concentration (grams per liter) was also measured by a STA-R coagulation analyzer.¹¹

Samples were sent to SomaLogic and measured by the SomaScan platform. The instrument measured 1310 total proteins, of which 24 proteins failed the quality check and were flagged. We selected eight VTE biomarkers that were measured by laboratory instruments and successfully measured by SomaScan: D-dimer; prothrombin; protein C; protein S; antithrombin; fibrinogen; and coagulation factors IX and XI. One control sample that failed quality control was excluded.

2.2 | Analysis Plan

To compare the agreement and interchangeability of the different measures we used the 95% agreement statistical method.¹² Since SomaScan uses relative fluorescence units as measures for protein concentration, and the laboratory instruments measure absolute

protein concentrations or activity (international units per milliliter), we applied an alternative method to assess agreement if measurements are on different units, as described by Bland and Altman.¹² First, we performed a linear regression per biomarker with laboratory instrument measures as the outcome and SomaScan measures as the independent variable. Second, we used the regression models to predict estimates of the laboratory instrument values using SomaScan values. After checking the normality of the residuals, we log-transformed the D-dimer measurements, as their distributions were very skewed. Finally, we calculated the 95% prediction interval (PI) to represent the equivalent of 95% limits of agreement.¹² This method is equivalent to comparing the mean differences of the two measurement methods. If the bias is consistent and the mean difference is close to zero, the result would show narrow prediction intervals. Consequently, the two methods would be interchangeable and in good agreement.¹³ It is difficult to define hard cutoff points for the intervals. Therefore, judging the agreement is considered a clinical question rather than a statistical one.¹⁴

3 | DISCUSSION AND RESULTS

We examined the agreement of SomaScan measurements of VTE biomarkers with the laboratory instruments. The table and figures for the results are shown in Table 1 and Figure 1. Although a particular biomarker may seem to be in good agreement due to oblique slopes, the appropriate indicator for agreement is the width of the prediction interval around the average fit of the regression line.¹²

Overall, the results indicate poor agreement of SomaScan with the validated laboratory instruments. The narrowest prediction interval, and thus the best agreement, were observed for antithrombin

TABLE 1 Average fit and average prediction intervals for SomaScan and laboratory instruments for the coagulation factors

Protein name	Units	Average fit (average 95% PI)	Average width ^b
Coagulation factor XI	%, 100% =1 IU/mL	124.3 (75.0-173.5)	98.5
Protein S	%, 100% =1 IU/mL	101.4 (80.2-122.7)	42.6
Protein C	%, 100% =1 IU/mL	133.9 (106.4-161.4)	55.1
Antithrombin	%, 100% =1 IU/mL	105.5 (91.0-120.1)	29.1
Coagulation factor IX	%, 100% =1 IU/mL	129.6 (81.0-178.2)	97.2
Prothrombin	(%) 100% =1 IU/ml	103.7 (80.3-127.1)	46.9
D-dimer			
Log	Log (ng/mL ^a)	6.2 (4.7-7.6)	2.9
Back-transformed	ng/mL ^a	492.7 (110.0-1998.2)	1888.2
Fibrinogen	g/L	3.3 (2.0-4.7)	2.6

Note: Activity of coagulation factor XI, protein S, protein C, antithrombin, coagulation factor IX, and prothrombin were measured by the same instrument and use international units per milliliter. D-dimer and fibrinogen total concentrations were measured by immunoassay instruments.

Abbreviation: PI, prediction interval.

^aD-dimer was assayed using the Vidas D-dimer assay. Unit type used was fibrinogen equivalent unit (500 ng FEU/mL = 250 ng D-dimer/mL).

^bAverage width: the average difference between the lower and upper limits of the prediction interval.

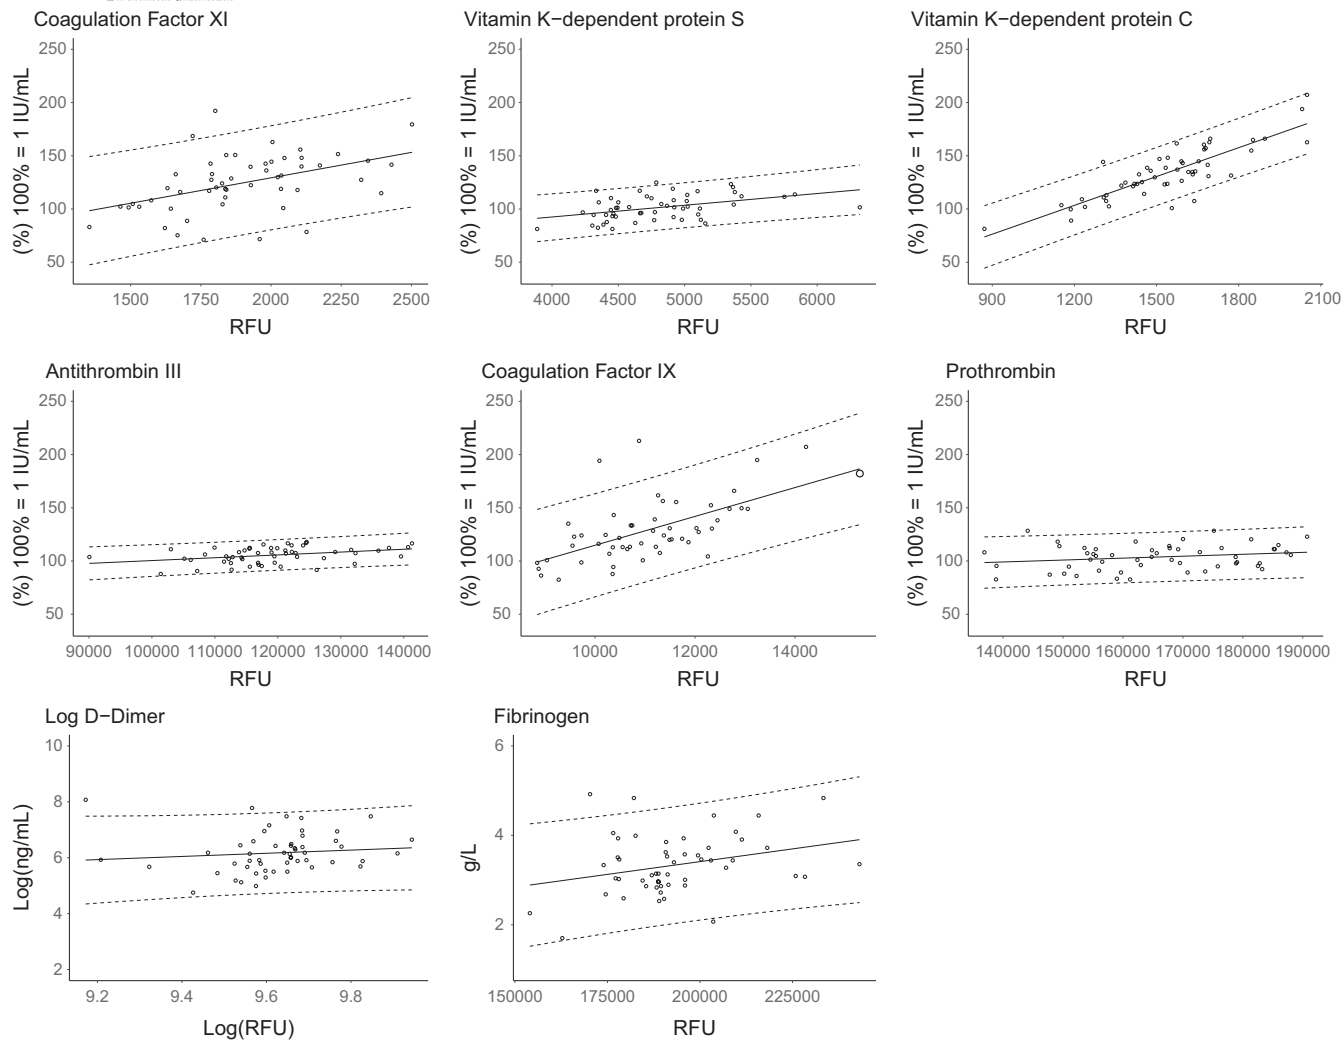


FIGURE 1 95% limits of agreement plots for each VTE biomarker. Narrow prediction intervals indicate higher agreement between the SomaScan (x axis) and laboratory instruments (y axis). Antithrombin had the narrowest interval and, therefore, the best agreement. D-dimer had the poorest agreement as indicated by the wide interval in the log-transformed plot. RFU: relative fluorescence units

(average fit, 105.52 IU/mL; 95% PI, 90.98-120.06) followed by protein S (average fit, 101.44 IU/mL; 95% PI, 80.15-122.73), prothrombin (average fit, 103.7 IU/mL; 95% PI, 80.27-127.13), and protein C (average fit, 133.87 IU/mL; 95% PI, 106.35-161.4). Factor IX (average fit, 129.62 IU/mL; 95% PI, 81.03-178.21) and factor XI (average fit, 124.26 IU/mL; 95% PI, 75-173.53) had a wide mean prediction interval and low agreement. The prediction interval for fibrinogen also had a wide interval (average fit, 3.3 g/L; 95% PI, 2.0-4.7). This result indicates that the predicted value of fibrinogen was within a prediction range (average width) of 2.6 g/L (~80%) of the laboratory measurement. Considering the wide prediction interval and the fact that the normal range of fibrinogen is between 2 and 5 g/L,¹⁵ we concluded that the SomaScan measurements of fibrinogen are in poor agreement with the laboratory instrument. Finally, agreement between SomaScan and laboratory instruments for D-dimer had the widest average interval (average fit, 6.2; 95% PI, 4.7-7.6) among the measured markers, as shown in Figure 1. The values and width of the interval for the log D-dimer plot may seem normal compared to the plots of the other measurements. However, unlike the other

biomarkers, D-dimer was measured in nanogram-per-milliliter units and was log-transformed to fulfill the requirement of normality for the analysis. After back-transforming the values, the agreement was very poor, as indicated by the extremely wide prediction interval (average fit, 492.7 ng/mL; 95% PI, 110.0-1998.2).

The current study demonstrated poor agreement of SomaScan VTE measures with the laboratory instruments, particularly for D-dimer, which is a particularly important VTE biomarker,^{1,4,6} despite passing quality control. This poor agreement could explain the reported lack of association between SomaScan D-dimer measurement and the risk of DVT.¹⁶

Despite the advantages of SomaScan for high-throughput measurements, the observed disagreement could be due to some of the platform's shortcomings.¹⁷ Some factors that can affect binding affinity are aptamer cross reactivity, genetic variations, posttranslational modifications, and the complexity and stability of the target protein structure. Moreover, SomaScan measurements are quantitative and not qualitative and would not be able to detect qualitative defects in the analysis. It is important to note that our assessment

was only of the eight VTE biomarkers available in our study and cannot be generalized to the agreement of the remaining proteins measured by SomaScan for our data set.

Two previous studies assessed the association between SomaScan measurements and VTE single-nucleotide polymorphisms in the SomaScan protein genome-wide association study.^{8,10} Since several genetic loci associated with VTE biomarkers have previously been identified, multiple hits were expected. However, only factor XI and protein C measured by SomaScan were associated with three loci and one locus, respectively. The lack of genetic correlations with the SomaScan measures for the biomarkers further supports our findings of poor agreement.

Possible limitations of the study are the usage of activity measurements for biomarkers versus the relative concentration reported by SomaScan. However, both D-dimer and fibrinogen showed poor agreement despite being measured as concentration measures. Moreover, viscosity-based activity measurements, such as the STA-R analyzer used here, are considered the standard for VTE studies.¹⁸⁻²⁰ Furthermore, the recommended sample size for Bland-Altman methods is usually $N > 100$.²¹ Our small size may affect the accuracy of the width of the 95% agreement intervals. However, we found that the agreement is very poor for some of the biomarkers, such as D-dimer, which cannot be fully explained by the sample size. Finally, it is unlikely the storage time of the plasma samples before the SomaScan analysis caused major degradation. Since the blood was collected, the samples were stored at -80°C , and the sampled aliquots were used for the primary analysis. Afterwards, the samples were not thawed until the analysis by SomaScan 5 years later. Several studies have shown that these conditions were optimal for the storage of plasma samples and maintain minimal degradation.²²⁻²⁴ Therefore, storage time and conditions are an unlikely cause to the disagreement in our results. Nevertheless, comparing the agreement of SomaScan with total concentrations for the other biomarkers and in larger studies may provide further insight.

4 | CONCLUSION

The 95% limit agreement is a simple and effective statistical method for comparing measurements by different methods. We believe it is important to apply this type of analysis to compare the measurements of exciting novel high-throughput platforms with current established measurements; thereby limiting measurement errors from affecting the results and conclusions based on such platforms.

In conclusion, despite the promising applications of aptamers for proteomics studies, we found that the applied SomaScan platform is not interchangeable with validated laboratory instruments for the VTE markers in our study. Therefore, caution is needed when applying SomaScan measurements for hypothesis-driven VTE studies using these markers. Whether this is also true for other biomarkers for VTE remains to be determined. It is clear that more studies of agreement with larger sample size and additional markers are needed.

ACKNOWLEDGMENTS

The authors thank the director of the anticoagulation clinic of Leiden, The Netherlands (F. J. M. van der Meer), who made the recruitment of patients in Leiden possible. L. Willems of Brillman is thanked for performing interviews and blood draws. I. de Jonge is thanked for her administrative support and data management. We are grateful to P. Noordijk, L. Mahic, and A. Hoenderdos for sample processing and laboratory analysis.

RELATIONSHIP DISCLOSURE

TB has received honoraria for consultancy from Organon Teknika and bioMerieux. DO Mook-Kanamori is a part-time clinical research consultant for Metabolon, Inc. All other authors declare no conflicts of interest.

AUTHOR CONTRIBUTIONS

TF designed the study and analyzed and drafted the manuscript. AvHV conceived and designed the study, acquired the data, obtained funding, and supervised the study. KWvD and DOM-K conceived, supervised, and designed the study. TB acquired the data and supervised the study. FRR supervised the study. All authors reviewed the manuscript.

ORCID

Tariq Faquih  <https://orcid.org/0000-0001-8026-2251>

TWITTER

Tariq Faquih  @TariqFaquih

Dennis O. Mook-Kanamori  @MookKanamori

REFERENCES

1. Heit JA. Epidemiology of venous thromboembolism. *Nat Rev Cardiol.* 2015;12(8):464-474.
2. Naess IA, Christiansen SC, Romundstad P, Cannegieter SC, Rosendaal FR, Hammerstrom J. Incidence and mortality of venous thrombosis: a population-based study. *J Thromb Haemost.* 2007;5(4):692-699.
3. Halaby R, Popma CJ, Cohen A et al. D-dimer elevation and adverse outcomes. *J Thromb Thrombolysis.* 2015;39(1):55-59.
4. Konstantinides SV, Meyer G, Becattini C et al. 2019 ESC Guidelines for the diagnosis and management of acute pulmonary embolism developed in collaboration with the European Respiratory Society (ERS): The Task Force for the Diagnosis and Management of Acute Pulmonary Embolism of the European Society of Cardiology (ESC). *Eur Heart J.* 2019;41(4):543-603.
5. Cristea IM, Gaskell SJ, Whetton AD. Proteomics techniques and their application to hematology. *Blood.* 2004;103(10):3624-3634.
6. Pabinger I, Ay C. Biomarkers and venous thromboembolism. *Arterioscler Thromb Vasc Biol.* 2009;29(3):332-336.
7. Gold L, Ayers D, Bertino J et al. Aptamer-based multiplexed proteomic technology for biomarker discovery. *PLoS One.* 2010;5(12):e15004.
8. Suhre K, Arnold M, Bhagwat AM et al. Connecting genetic risk to disease end points through the human blood plasma proteome. *Nat Commun.* 2017;8:14357.
9. Ganz P, Heidecker B, Hveem K et al. Development and validation of a protein-based risk score for cardiovascular

- outcomes among patients with stable coronary heart disease. *JAMA*. 2016;315(23):2532-2541.
10. Sun BB, Maranville JC, Peters JE et al. Genomic atlas of the human plasma proteome. *Nature*. 2018;558(7708):73-79.
 11. van Hylckama VA, Baglin CA, Luddington R, MacDonald S, Rosendaal FR, Baglin TP. The risk of a first and a recurrent venous thrombosis associated with an elevated D-dimer level and an elevated thrombin potential: results of the THE-VTE study. *J Thromb Haemost*. 2015;13(9):1642-1652.
 12. Bland JM, Altman DG. Applying the right statistics: analyses of measurement studies. *Ultrasound Obstet Gynecol*. 2003;22(1):85-93.
 13. Giavarina D. Understanding Bland Altman analysis. *Biochem Med*. 2015;25(2):141-151.
 14. Bland JM. Interpreting the limits of agreement: do I have good or bad agreement? 2009 [updated March 20, 2009]. Available from: <https://www-users.york.ac.uk/~mb55/meas/interlim.htm>. Accessed January 11, 2021.
 15. Kattula S, Byrnes JR, Wolberg AS. Fibrinogen and fibrin in hemostasis and thrombosis. *Arterioscler Thromb Vasc Biol*. 2017;37(3):e13-e21.
 16. Tala JA, Polikoff LA, Pinto MG et al. Protein biomarkers for incident deep venous thrombosis in critically ill adolescents: an exploratory study. *Pediatr Blood Cancer*. 2020;67(4):e28159.
 17. Joshi A, Mayr M. In aptamers they trust: the caveats of the SomaScan biomarker discovery platform from SomaLogic. *Circulation*. 2018;138(22):2482-2485.
 18. Justine B, Thomas S, Bruno P, Marc GB, Anne-Françoise S-S, Aurélien L. Évaluation des performances de l'automate STA R Max®(Stago) pour les paramètres d'hémostase de routine. *Ann Biol Clin*. 2018;76(2):143-149.
 19. Flanders MM, Crist R, Safapour S, Rodgers GM. Evaluation and performance characteristics of the STA-R coagulation analyzer. *Clin Chem*. 2002;48(9):1622-1624.
 20. Cupaiolo R, Govaerts D, Blauwaert M, Cauchie P. Performance evaluation of a new Stago® automated haemostasis analyser: the STA R Max® 2. *Int J Lab Hematol*. 2019;41(6):731-737.
 21. Bland JM. How can I decide the sample size for a study of agreement between two methods of measurement? 2004 [updated January 12, 2004]. Available from: <https://www-users.york.ac.uk/~mb55/meas/sizemeth.htm>. Accessed January 1, 2021.
 22. Hubel A, Spindler R, Skubitz AP. Storage of human biospecimens: selection of the optimal storage temperature. *Biopreserv Biobank*. 2014;12(3):165-175.
 23. Tworoger SS, Hankinson SE. Collection, processing, and storage of biological samples in epidemiologic studies: sex hormones, carotenoids, inflammatory markers, and proteomics as examples. *Cancer Epidemiol Biomarkers Prev*. 2006;15(9):1578-1581.
 24. Wagner-Golbs A, Neuber S, Kamlage B et al. Effects of long-term storage at -80 °C on the human plasma metabolome. *Metabolites*. 2019;9(5):99.

How to cite this article: Faquih T, Mook-Kanamori DO, Rosendaal FR, Baglin T, Willems van Dijk K, van Hylckama Vlieg A. Agreement of aptamer proteomics with standard methods for measuring venous thrombosis biomarkers. *Res Pract Thromb Haemost*. 2021;5:e12526. <https://doi.org/10.1002/rth2.12526>