



Universiteit
Leiden
The Netherlands

Electroextraction approaches for preconcentration of metabolites

Oedit, A.

Citation

Oedit, A. (2023, March 22). *Electroextraction approaches for preconcentration of metabolites*. Retrieved from <https://hdl.handle.net/1887/3576693>

Version: Publisher's Version

License: [Licence agreement concerning inclusion of doctoral thesis in the Institutional Repository of the University of Leiden](#)

Downloaded from: <https://hdl.handle.net/1887/3576693>

Note: To cite this publication please use the final published version (if applicable).

Chapter 3

Lab-on-a-Chip hyphenation with mass spectrometry: strategies for bioanalytical applications

Based on:

Amar Oedit, Paul Vulto, Rawi Ramautar, Peter W. Lindenburg and Thomas Hankemeier

**Lab-on-a-Chip hyphenation with mass spectrometry: strategies
for bioanalytical applications**

Current Opinion in Biotechnology **31**, 79 – 85, (2015)


Highlights

- The state-of-the-art of coupling Lab-on-a-Chip to mass spectrometry is provided
- Applications using Lab-on-a-Chip coupled to mass spectrometry are discussed
- We look at the role of miniaturized analysis systems in the analytical workflow
- Perspective on integration of miniaturized analytical systems in the lab is provided

Abstract

The Lab-on-a-Chip concept aims to miniaturize laboratory processes to enable automation and/or parallelization via microfluidic chips that are capable of handling minute sample volumes. Nowadays, mass spectrometry is the detection method of choice, because of its selectivity, sensitivity and wide application range. We review the most interesting examples over the last two-and-a-half years where the two techniques were used for bioanalytical applications. Furthermore, we discuss the merits and limitations of such hyphenated systems. We inventorize the reported applications and approaches. We see an ongoing trend towards chip-based liquid chromatography – mass spectrometry usage, small volume analysis applications, particularly in the field of proteomics where bottom-up approaches profit from chip-based technologies and hyphenation with complex cell cultures.

Graphical Abstract

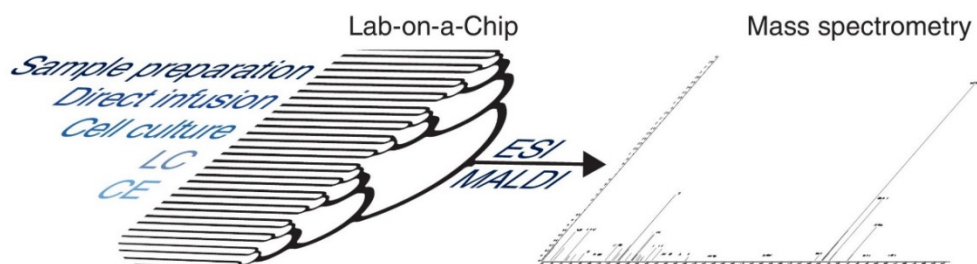

Introduction

Current day challenges in bioanalysis include automation, throughput, small volume handling and disposability. These challenges are addressed with increasing success through miniaturized laboratory processes, so-called Lab-on-a-Chip (LOC). LOC systems use microfluidics (see Supporting Information) to handle minute volumes and can be manufactured as cost-effective disposables. Moreover, it is possible to integrate laboratory protocols and/or analysis methods into a single cartridge.

Typical detection techniques that are combined with LOC techniques include optical detection (*e.g.*, UV/Vis spectrophotometry), nuclear magnetic resonance, and electrochemical detection¹. To date, none of these sensing techniques can match the selectivity and sensitivity of mass spectrometry (MS).

LOC systems and MS match particularly well. LOC operates in the small volume domain and provides (limited) separation. MS detection improves when downscaled, it has a high resolving power and is sensitive.

One of the first hyphenated LOC-MS systems was reported by Xue *et al.*². At the time a key driver for this combination was to increase throughput in diagnostics and screening applications by using multiple fluidic channels and ionization sprays. The authors also perceived the potential for sample preparation, capillary electrophoresis (CE) and liquid chromatography (LC) on chip coupled to MS.

We inventorized developments in the last 2.5 years before publication in the LOC-MS field from two perspectives: analytical approach (Figure 1a) and application area (Figure 1b). The most commonly used approach is LC and the most commonly used application area is proteomics. The review is structured on approaches to sample preparation, direct infusion MS, separation and the total analysis system principle. Comprehensive reviews on LOC-MS have recently been published by Gao *et al.*^{3*} and Feng *et al.*^{4*}. In this critical review we argue that the combination LOC and MS will prove to be the ideal combination for bioanalytical applications and we discuss the, in our view, crucial steps forward and the most dominant trends.

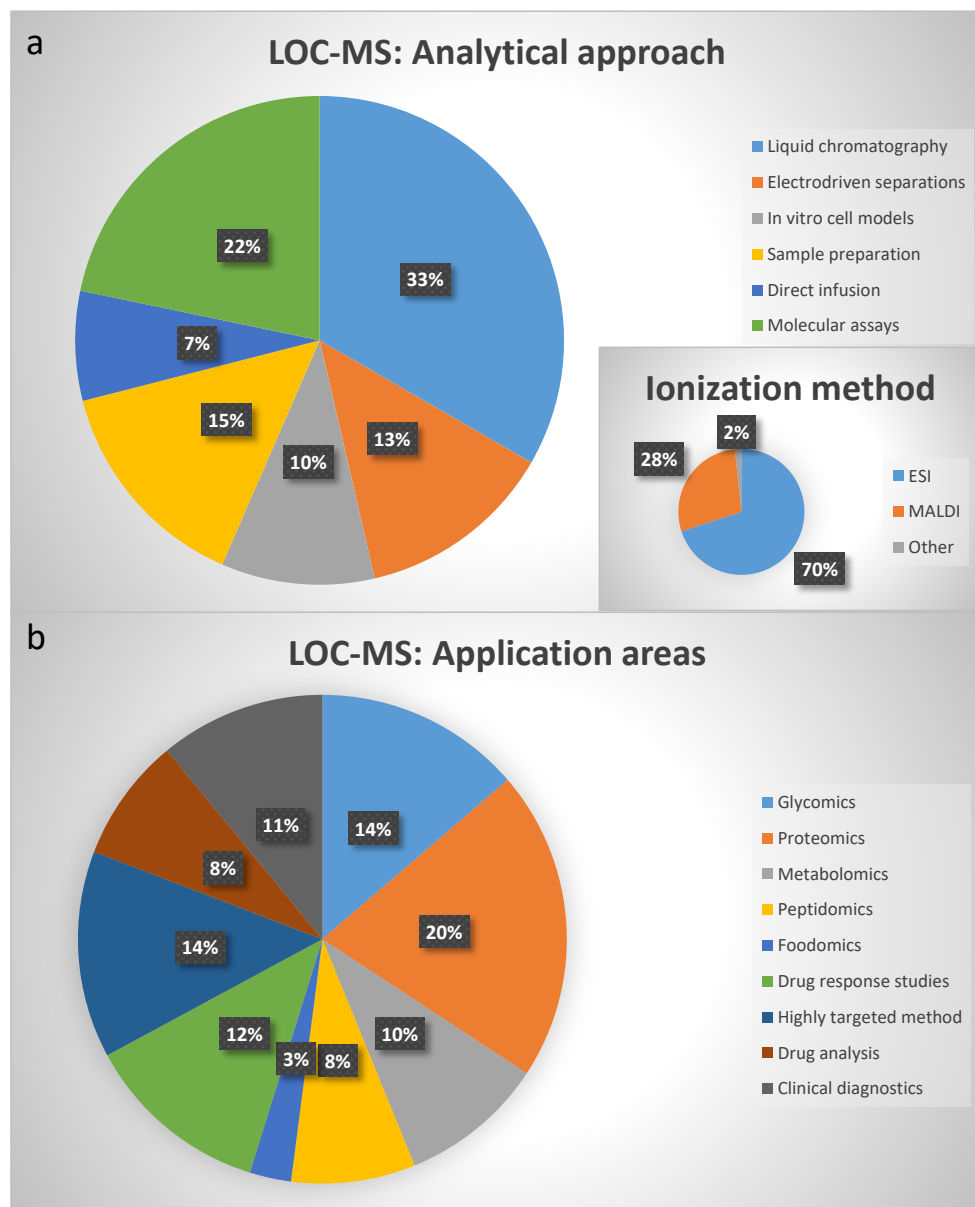


Figure 1. Overview of LOC-MS publications in the last 2.5 years before publication, based on approach and application area of LOC-MS hyphenated techniques. A total of 192 papers published between January 1st 2012 and June 1st 2014 were found using the following query on PubMed “((((microfluidic*) OR lab-on-a-chip) AND mass spectromet*)) AND (“2012”[Date - Publication]: “2014”[Date - Publication])”, of these 68 were research papers within the scope of this review. These articles were categorized and included in this figure, several articles had multiple classifications. **(a)** A pie chart of published works describing various analytical approaches that were hyphenated to mass spectrometry. The insert provides an overview of the type of ionization sources used. **(b)** A pie chart of research application areas that use LOC-MS.

Sample preparation

Common sample preparation techniques are liquid-liquid extraction and solid-phase extraction; only one example of the latter was reported on LOCs in the last 2.5 years before publication. Solid-phase extraction was integrated with *in vitro* cell culturing and will be discussed later in the review. In bottom-up proteomics proteolysis is an important part of the sample preparation workflow; the majority of LOCs focused on this.

Several devices integrating the proteomics workflow into one LOC were presented. One example is a fully integrated electrowetting-powered LOC capable of automated performance of the whole proteomics workflow (from sample preparation to acquisition). MALDI was enabled by removing the top cover of the LOC after addition of the MALDI matrix. Then the open LOC was placed into a custom-made MALDI plate and analysis was performed⁵. A device with similar functionality was created using Quake valves to generate and control droplets in an LOC coupled to MS via an integrated nano-ESI emitter⁶. Furthermore, a droplet microarray plate for the proteomics workflow was developed. This microarray was interfaced to ESI-MS via an L-shaped capillary with a tapered tip that served as sampling probe and ESI source⁷. Tryptic digestion for proteomics after LC-based fractionation is normally performed off-line and suffers from low throughput. On-line methodologies involving immobilized trypsin have aspecific adsorption, which leads to carry-over. These problems were solved via an LOC in which LC effluent droplets were trypsinized and consequently quenched. The LOC was interfaced to MS via an integrated stainless steel emitter⁸. Another device interfaced droplet microfluidics with a microarray plate containing hydrophilic and hydrophobic spots for the observation of enzyme kinetics (angiotensin II to angiotensin I conversion) in a massive parallel format – 8265 droplets were deposited on the plate – as shown in Figure 2d – and dried using N₂. Afterwards MALDI matrix was deposited and, because each dried spot represents a time-point, the reaction kinetics could be observed via MALDI-MS⁹. An LOC with an integrated proteolysis microreactor to monitor hydrogen-deuterium exchange in proteins was coupled to MS via a custom ESI emitter for both continuous¹⁰ and pulse¹¹ labelling experiments, enabling the characterization of conformational changes that cannot be probed by conventional techniques. In this work, a push-pull probe was coupled to ESI-MS and a droplet micro-array. This probe was used to analyze dry surfaces via both scanning electrochemical microscopy and droplet deposition on a MALDI

plate. It was also used to image immobilized enzymes under a fluid layer by delivering para-aminophenyl phosphate via the microfluidic probe and analyzing the para-aminophenol products by ESI-MS (see also figure 2b)¹². An application where electrowetting-based LOCS are applied in combination with ESI-MS is dried blood spot screening (DBS). Succinylacetone in DBS samples was quantified using a fully automated, nine-step analysis on an LOC. Interfacing to MS was achieved via a removable pulled glass capillary emitter nano-ESI source, inserted between the chip substrates. No statistically significant differences (95% confidence interval) were found between results obtained with conventional methods and the LOC¹³.

Direct infusion-MS

Direct infusion-MS (DI-MS) refers to introducing sample into the MS without prior separation. DI-MS chips are marketed by Advion. These systems are capable of delivering robust data, can be used for high-throughput analyses, and utilize disposable tips, thereby removing carry-over. Recently it has been used for ganglioside analysis from the human caudate nucleus¹⁴, DBS alpha-galactosidase assaying to diagnose Fabry's disease¹⁵ and determination of unusual glycosaminoglycans sulphation patterns in murine brain tissue¹⁶. A competitor for this system is the capillary gap sampler (Figure 2e). Analyte droplets are introduced from a 384-well plate into a liquid junction between a glass capillary supply line and ESI needle¹⁷. The main advantage of this system is its ability to sample nanoliters, which is a three-order magnitude improvement over the Advion system.

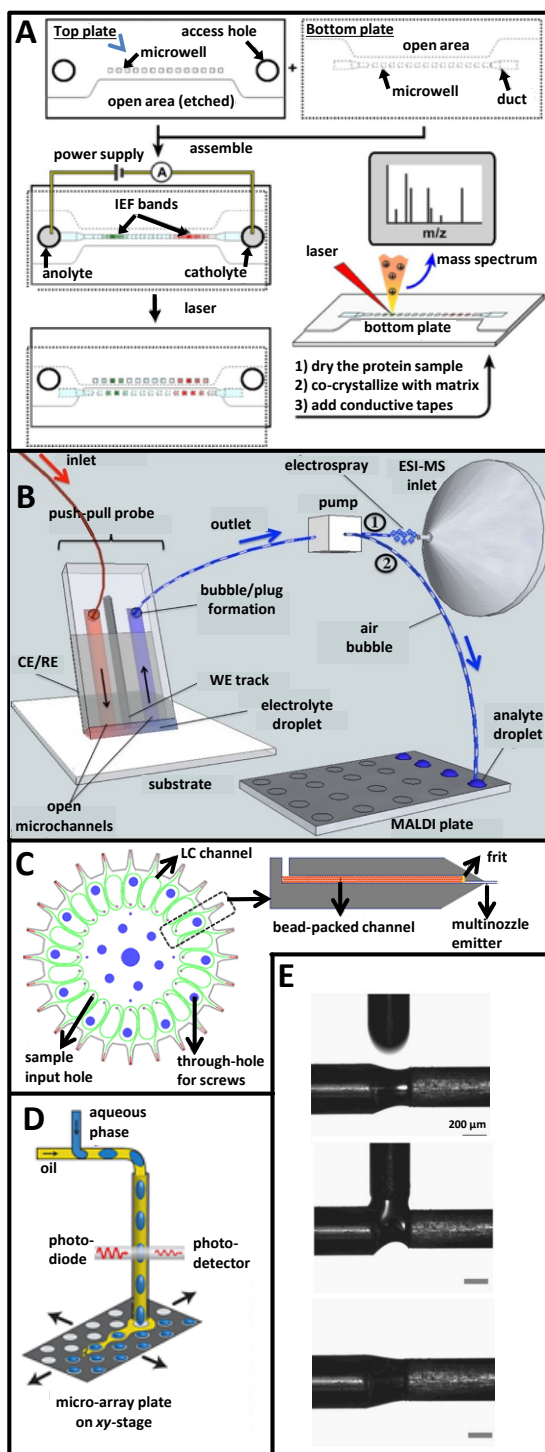


Figure 2. Developments in hyphenated LOC MS techniques: **(a)** 'SlipChip' based iso-electric focussing hyphenated with MS. The top and bottom chip substrates of each contain microfluidic structures that combined create a microfluidic path. After IEF is performed a slipping operation is performed to disconnect the fluidic path. Separated proteins and metabolites analytes are dried and co-crystallized with MALDI matrix, followed by detection via MALDI-MS. Reprinted with permission³⁹. **(b)** Microfluidic push-pull probe for the scanning of dry surfaces. The push-pull probe immerses the dry sample with an electrolyte and electrochemical measurements are carried out on one nanoliter of electrolyte. The flow is segmented by air bubbles that are introduced at the junction between the probe and the outlet capillary. After that the droplets are spotted on a MALDI plate for analysis or sent to an ESI source. Reprinted with permission¹². **(c)** Multinozzle emitter array chip for parallel analyses. The chip consists of 24 channels (which are optionally packed with LC column material) each connected with an emitter. Modified with permission³³. **(d)** Droplet microfluidic dispensing interface for MALDI analysis. Droplets are dispensed on a micro-array plate containing hydrophilic (26444) and hydrophobic areas. After deposition the oil phase quickly evaporates. Enzymatic reactions can be monitored over time by spotting droplets and drying them with nitrogen gas followed by deposition of MALDI matrix for MALDI analysis over time. Modified with permission⁹. **(e)** Capillary gap sampler for direct analysis of small volume samples. Nanoliters of sample are introduced from a 384-well plate via a liquid junction suspended in between a fused silica buffer supply line and a stainless steel ESI emitter. Modified with permission⁴⁷.

Separation

Chip-based liquid-chromatography

The vast majority of papers reporting the use of chip-based LC (chipLC) utilized commercial systems, for example from Agilent Technologies, Waters Corporation and Eksigent. Miniaturized LC-MS exists in a variant known as nanoLC-MS, which provides extremely sensitive analysis, but can have issues with robustness due to dead volumes and leaks. ChipLC offers a solution for these challenges.

ChipLC interfacing to MS is often achieved via tubing to ESI sources or on-chip integrated sprayers coupled to a (special) interface. Monolithically integrated sprayers are also emerging¹⁸. ChipLC-MS has been used for, amongst others: pharmacokinetic studies in rodents¹⁹⁻²¹, detecting aflatoxins in peanut products²², detecting gangliosides and sulfatides in murine brains²³, glycomic²⁴ and proteomic biomarker discovery²⁵, quantification of matrix metalloprotease-9 in bronchoalveolar lavage fluid²⁶ and quantification of stable isotope dimethyl-labelled phosphopeptides²⁷. ChipLC-MS steroid analysis^{28,29} demonstrated improved LOD compared to conventional LC-MS. ChipLC was also coupled to MALDI-MS, using EOF-based pumps. After separation the proteins were transported orthogonally via electroosmosis in microchannels to MALDI reservoirs³⁰. Another important development is that, to our knowledge, chipLC-MS was used for the first time on patient samples in a phase II clinical trial. ChipLC-MS was used to monitor incorporation of deuterated leucine into an apolipoprotein(a)-derived peptide³¹. This indicates that chipLC-MS is currently at a level of robustness that pharmaceutical companies are willing to employ it during drug development.

Other significant developments indicate maturation of chipLC-MS are the appearance of validated chipLC-MS methods for analysis of illegal drugs³², monitoring of fluoxetine and norfluoxetine in rat serum¹⁹ and 7-ethy-10-hydroxycampothecin in murine plasma²⁰. A commercial application by Newomics Inc. is the multinozzle emitter array chip (Figure 2c), which can be used for parallel DI protein analysis and enhanced throughput chipLC-MS analysis of tryptic digests, thanks to parallelization enabled by the multiple nozzles per emitter³³.

Electro-driven separations

The main challenge in chip-based electrodriven separation systems lies in MS interfacing. Recent chip-based capillary electrophoresis (chipCE) works have focused on increasing the robustness of interfacing to MS, for example through monolithic integration of ESI tips^{34,35}. Also, an integrated make-up flow chip design and its effect on separation, LOD and robustness of amino acid analysis was demonstrated³⁶. Furthermore, chips utilizing zero, one and three make-up flows were compared. The authors conclude that, while LODs for cardiac drugs are improved without make-up flow, the LOCs with make-up flow are more robust and easier optimized³⁷.

Optimal chipCE-MS conditions for proteins and peptides are challenging: a low ionic strength background electrolyte and acidic pH are required for efficient ESI. Under these conditions silica is prone to electro-osmotic flow (EOF) instability due to protein-wall interactions. Batz *et al.* coated silica channel walls with aminopropyl silanes, ensuring stable EOF between pH 2.8 and 7.5, and an inter-device EOF reproducibility of 2.6% RSD. Protein analysis showed 0.7% RSD migration time reproducibility and plate numbers up to 400.000; peptide separation efficiency was over 600.000, the highest reported for any CE-ESI-MS. ESI was achieved from the corner of the chip aided by electroosmosis-driven make-up flow³⁸.

In another electro-driven separation, capillary isoelectric focusing (cIEF), ampholytic analytes are separated according to their isoelectric point in a pH gradient. Wang *et al.* developed a methodology to hyphenate chip-IEF to MS using nanowells in glass bottom and top plates, which, when oriented in a semi-overlapping fashion, form a separation channel (Figure 2a). After separation the glass plates were moved, resulting in MALDI-MS-ready nanowells containing separated analytes. Eleven amine metabolites were putatively identified in CSF using this method³⁹.

Li *et al.* integrated cell culturing and chiral chipCE-MS analysis in one LOC. Cell culturing was performed on a 0.22 μm filter on top of the sample inlet channel; downstream the separation channel, chiral selectors (moving opposite to the net flow) were introduced and the extracellular matrix was sampled periodically. ESI took place at corner of the chip, aided by a make-up flow. The enantioselective catabolism of racemic DOPA by neuronal cells was monitored⁴⁰, showing that chipCE is a feasible technique for analysis of *in vitro* cell models.

Towards integrated total analysis systems

Hyphenating *in vitro* cell models to MS is attractive as the information level provided by MS exceeds traditional optical detection techniques. Furthermore, on-line analysis allows following kinetics. Several LOC devices integrating cell culture and sample preparation have been developed by the Jin-Ming Lin group. In these devices, micro-solid phase extraction is integrated. The interfacing to MS is achieved via tubing connected to an ESI needle. Applications include: measuring acetaminophen metabolism via cultured microsomes⁴¹, quantitative analysis of tumor cell metabolism of genistein⁴², testing of absorption of various concentrations of methotrexate and its cytotoxic effects⁴³ and the uptake of curcumin by CaCo2-cell lines⁴⁴. One system was used for studying signaling molecules in cell-cell communications⁴⁵. Emerging trends involving 3D cell culture and organ-on-a-chip will likely increase the attention for these types of systems.

Outlook and conclusion

An overview incentives and pre-requisites for adoption of LOC-MS systems is presented in Table 1. The incentives to use LOC-MS are to enable small volume analysis, high throughput/parallelization and automation, time-continuous monitoring and on-line sample preparation. Several of these pre-requisites have already been fulfilled. Commercialized systems as well as cartridge-integrated set-ups are present especially in the chipLC-MS field. The added value and benefit are clear, especially in the proteomics field. The perfect match between the scaling efficiencies of enzymatic reactions with the decreasing volumes provided by droplet-sized microreactors, proteomics, and MS' ability to deal with low-volume samples make it an ideal candidate for wide-spread usage within the proteomics community. However, robust datasets, *i.e.*, analysis of sample series, are demonstrated sparsely, one example being continuous monitoring of enzyme kinetics on a micro-array plate.

Table 1. Overview of incentives and pre-requisites for the adoption of LOC-MS devices.

Incentives	Examples
Small volume analysis	Single cell analysis, neonate screening, animal model fluids and tissues, all direct infusion and separation approaches, trace analysis, push pull probe, capillary gap sampler, clinical diagnostics and drug screening
High throughput, parallelization and automation	Drug screening (<i>in vitro</i> and assay-based), sample preparation in proteomics, DBS analysis, multinozzle emitter array, Advion systems, capillary gap sampler
Time-continuous monitoring	<i>In vitro</i> cell models, enzymatic assays
Molecular interaction assays	Enzyme reactions, frontal affinity chromatography, H/D exchange
On-line sample preparation	On-line proteolysis, integrated proteomic workflows

Pre-requisites

Robust datasets

Standardization and protocols

Clear added value and benefit

Cartridge integration / 'Plug and play'

Commercialization of set-ups

We foresee the usage of chipLC-MS becoming commonplace in the upcoming years, especially since several commercial systems that offer increased throughput, sensitive analysis and allow easy operation are already available. The main advantage of chipLC-MS lies in its reduced sample usage and therefore it will be predominantly used for small sample volume applications. ChipCE-MS systems need further improvements in robustness before they can be applied on a larger scale. Work is currently focused on make-up flows, which we expect to lead to more robust systems.

Lastly, we foresee increasing attention for coupling *in vitro* cell models (such as organ-on-a-chip and 3D cell culture) to MS. Pharmaceutical companies are increasingly interested to make use of such devices to gain additional information efficacy and toxicity of their compounds in the discovery and pre-clinical stage.

References and recommended reading

Papers of particular interest, published within the period of review, have been highlighted as:

- of special interest
- of outstanding interest

Acknowledgements

We would like to express our gratitude to Vincent van Duinen for the creation of the graphical abstract.

This work was made possible by the European Union STATegra project, EU FP7 grant number 30600.

References

- 1 Zhu, Y. & Fang, Q. Analytical detection techniques for droplet microfluidics--a review. *Analytica chimica acta* **787**, 24-35, doi:10.1016/j.aca.2013.04.064 (2013).
- 2 Xue, Q. *et al.* Multichannel microchip electrospray mass spectrometry. *Anal Chem* **69**, 426-430 (1997).
- 3•• Gao, D., Liu, H., Jiang, Y. & Lin, J. M. Recent advances in microfluidics combined with mass spectrometry: technologies and applications. *Lab Chip* **13**, 3309-3322, doi:10.1039/c3lc50449b (2013).
- 4•• Feng, X., Liu, B. F., Li, J. & Liu, X. Advances in coupling microfluidic chips to mass spectrometry. *Mass spectrometry reviews*, doi:10.1002/mas.21417 (2014).
- 5 Aijian, A. P., Chatterjee, D. & Garrell, R. L. Fluorinated liquid-enabled protein handling and surfactant-aided crystallization for fully in situ digital microfluidic MALDI-MS analysis. *Lab Chip* **12**, 2552-2559, doi:10.1039/c2lc21135a (2012).
- 6 Sun, X., Tang, K., Smith, R. D. & Kelly, R. T. Controlled dispensing and mixing of pico- to nanoliter volumes using on-demand droplet-based microfluidics. *Microfluid Nanofluidics* **15**, 117-126, doi:10.1007/s10404-012-1133-1 (2013).
- 7 Su, Y., Zhu, Y. & Fang, Q. A multifunctional microfluidic droplet-array chip for analysis by electrospray ionization mass spectrometry. *Lab Chip* **13**, 1876-1882, doi:10.1039/c3lc00063j (2013).
- 8 Ji, J. *et al.* Proteolysis in microfluidic droplets: an approach to interface protein separation and peptide mass spectrometry. *Lab Chip* **12**, 2625-2629, doi:10.1039/c2lc40206h (2012).
- 9• Kuster, S. K. *et al.* Interfacing droplet microfluidics with matrix-assisted laser desorption/ionization mass spectrometry: label-free content analysis of single droplets. *Anal Chem* **85**, 1285-1289, doi:10.1021/ac3033189 (2013).
- 10 Rob, T. *et al.* Measuring dynamics in weakly structured regions of proteins using microfluidics-enabled subsecond H/D exchange mass spectrometry. *Anal Chem* **84**, 3771-3779, doi:10.1021/ac300365u (2012).
- 11 Rob, T., Gill, P. K., Golemi-Kotra, D. & Wilson, D. J. An electrospray ms-coupled microfluidic device for sub-second hydrogen/deuterium exchange pulse-labelling reveals allosteric effects in enzyme inhibition. *Lab Chip* **13**, 2528-2532, doi:10.1039/c3lc00007a (2013).
- 12• Momotenko, D. *et al.* Electrochemical push-pull scanner with mass spectrometry detection. *Anal Chem* **84**, 6630-6637, doi:10.1021/ac300999v (2012).
- 13 Shih, S. C. *et al.* Dried blood spot analysis by digital microfluidics coupled to nanoelectrospray ionization mass spectrometry. *Anal Chem* **84**, 3731-3738, doi:10.1021/ac300305s (2012).
- 14 Serb, A. F., Sisu, E., Vukelic, Z. & Zamfir, A. D. Profiling and sequencing of gangliosides from human caudate nucleus by chip-nanoelectrospray mass spectrometry. *Journal of mass spectrometry : JMS* **47**, 1561-1570, doi:10.1002/jms.3116 (2012).
- 15 Flangea, C. *et al.* Testing the feasibility of fully automated chip-based nanoelectrospray ionization mass spectrometry as a novel tool for rapid diagnosis of Fabry disease. *Electrophoresis* **34**, 1572-1580, doi:10.1002/elps.201200665 (2013).
- 16 Flangea, C., Petrescu, A. J., Seidler, D. G., Munteanu, C. V. & Zamfir, A. D. Identification of an unusually sulfated tetrasaccharide chondroitin/dermatan motif in mouse brain by combining chip-nanoelectrospray multistage MS2 -MS4 and high resolution MS. *Electrophoresis* **34**, 1581-1592, doi:10.1002/elps.201200704 (2013).

- 17• Neu, V., Steiner, R., Muller, S., Fattinger, C. & Zenobi, R. Development and characterization of a capillary gap sampler as new microfluidic device for fast and direct analysis of low sample amounts by ESI-MS. *Anal Chem* **85**, 4628-4635, doi:10.1021/ac400186t (2013).
- 18 Sainiemi, L., Nissila, T., Kostianen, R., Franssila, S. & Ketola, R. A. A microfabricated micropillar liquid chromatographic chip monolithically integrated with an electrospray ionization tip. *Lab Chip* **12**, 325-332, doi:10.1039/c1lc20874h (2012).
- 19 Houbart, V. *et al.* A validated microfluidics-based LC-chip-MS/MS method for the quantitation of fluoxetine and norfluoxetine in rat serum. *Electrophoresis* **33**, 3370-3379, doi:10.1002/elps.201200168 (2012).
- 20 Ahn, G. *et al.* Development and validation of a microfluidic chip-based nano-liquid chromatography-triple quadrupole tandem mass spectrometry method for a sensitive and reliable quantification of 7-ethyl-10-hydroxycamptothecin (SN38) in mouse plasma. *Analytical and bioanalytical chemistry* **405**, 9817-9824, doi:10.1007/s00216-013-7411-2 (2013).
- 21 Gallagher, R. *et al.* The application of a new microfluidic device for the simultaneous identification and quantitation of midazolam metabolites obtained from a single micro-litre of chimeric mice blood. *Rapid communications in mass spectrometry : RCM* **28**, 1293-1302, doi:10.1002/rcm.6902 (2014).
- 22 Liu, H. Y., Lin, S. L., Chan, S. A., Lin, T. Y. & Fuh, M. R. Microfluidic chip-based nano-liquid chromatography tandem mass spectrometry for quantification of aflatoxins in peanut products. *Talanta* **113**, 76-81, doi:10.1016/j.talanta.2013.03.053 (2013).
- 23 Lee, H. *et al.* Multiple precursor ion scanning of gangliosides and sulfatides with a reversed-phase microfluidic chip and quadrupole time-of-flight mass spectrometry. *Anal Chem* **84**, 5905-5912, doi:10.1021/ac300254d (2012).
- 24 Hua, S. *et al.* Isomer-specific chromatographic profiling yields highly sensitive and specific potential N-glycan biomarkers for epithelial ovarian cancer. *J Chromatogr A* **1279**, 58-67, doi:10.1016/j.chroma.2012.12.079 (2013).
- 25 Franciosi, L. *et al.* Proteomic analysis of human epithelial lining fluid by microfluidics-based nanoLC-MS/MS: a feasibility study. *Electrophoresis* **34**, 2683-2694, doi:10.1002/elps.201300020 (2013).
- 26 Prely, L. M. *et al.* Quantification of matrix metalloprotease-9 in bronchoalveolar lavage fluid by selected reaction monitoring with microfluidics nano-liquid-chromatography-mass spectrometry. *J Chromatogr A* **1246**, 103-110, doi:10.1016/j.chroma.2012.02.076 (2012).
- 27 Polat, A. N., Kraiczek, K., Heck, A. J., Raijmakers, R. & Mohammed, S. Fully automated isotopic dimethyl labeling and phosphopeptide enrichment using a microfluidic HPLC phosphochip. *Analytical and bioanalytical chemistry* **404**, 2507-2512, doi:10.1007/s00216-012-6395-7 (2012).
- 28 Ahonen, L. *et al.* Comparison of liquid chromatography-microchip/mass spectrometry to conventional liquid chromatography-mass spectrometry for the analysis of steroids. *Analytica chimica acta* **721**, 115-121, doi:10.1016/j.aca.2012.01.039 (2012).
- 29 Broccardo, C. J. *et al.* Multiplexed analysis of steroid hormones in human serum using novel microflow tile technology and LC-MS/MS. *Journal of chromatography. B, Analytical technologies in the biomedical and life sciences* **934**, 16-21, doi:10.1016/j.jchromb.2013.06.031 (2013).
- 30 Lazar, I. M. & Kabulski, J. L. Microfluidic LC device with orthogonal sample extraction for on-chip MALDI-MS detection. *Lab Chip* **13**, 2055-2065, doi:10.1039/c3lc50190f (2013).

- 31 Zhou, H. *et al.* Measurement of apo(a) kinetics in human subjects using a microfluidic device with tandem mass spectrometry. *Rapid communications in mass spectrometry : RCM* **27**, 1294-1302, doi:10.1002/rcm.6572 (2013).
- 32 Zhu, K. Y. *et al.* Microfluidic chip based nano liquid chromatography coupled to tandem mass spectrometry for the determination of abused drugs and metabolites in human hair. *Analytical and bioanalytical chemistry* **402**, 2805-2815, doi:10.1007/s00216-012-5711-6 (2012).
- 33• Mao, P., Gomez-Sjoberg, R. & Wang, D. Multinozzle emitter array chips for small-volume proteomics. *Anal Chem* **85**, 816-819, doi:10.1021/ac3032965 (2013).
- 34 Sainiemi, L., Sikanen, T. & Kostianen, R. Integration of fully microfabricated, three-dimensionally sharp electrospray ionization tips with microfluidic glass chips. *Anal Chem* **84**, 8973-8979, doi:10.1021/ac301602b (2012).
- 35 Li, X., Xiao, D., Sanders, T., Tchounwou, P. B. & Liu, Y. M. Fast quantification of amino acids by microchip electrophoresis-mass spectrometry. *Analytical and bioanalytical chemistry* **405**, 8131-8136, doi:10.1007/s00216-013-7260-z (2013).
- 36 Li, X., Zhao, S. & Liu, Y. M. Evaluation of a microchip electrophoresis-mass spectrometry platform deploying a pressure-driven make-up flow. *J Chromatogr A* **1285**, 159-164, doi:10.1016/j.chroma.2013.02.031 (2013).
- 37 Schwarzkopf, F., Scholl, T., Ohla, S. & Belder, D. Improving sensitivity in microchip electrophoresis coupled to ESI-MS/MS on the example of a cardiac drug mixture. *Electrophoresis* **35**, 1880-1886, doi:10.1002/elps.201300615 (2014).
- 38 Batz, N. G., Mellors, J. S., Alarie, J. P. & Ramsey, J. M. Chemical vapor deposition of aminopropyl silanes in microfluidic channels for highly efficient microchip capillary electrophoresis-electrospray ionization-mass spectrometry. *Anal Chem* **86**, 3493-3500, doi:10.1021/ac404106u (2014).
- 39• Wang, S. *et al.* Interface solution isoelectric focusing with in situ MALDI-TOF mass spectrometry. *Electrophoresis*, doi:10.1002/elps.201400083 (2014).
- 40 Li, X., Xiao, D., Ou, X. M., McCullm, C. & Liu, Y. M. A microchip electrophoresis-mass spectrometric platform for fast separation and identification of enantiomers employing the partial filling technique. *J Chromatogr A* **1318**, 251-256 (2013).
- 41 Mao, S., Gao, D., Liu, W., Wei, H. & Lin, J. M. Imitation of drug metabolism in human liver and cytotoxicity assay using a microfluidic device coupled to mass spectrometric detection. *Lab Chip* **12**, 219-226, doi:10.1039/c1lc20678h (2012).
- 42 Chen, Q., Wu, J., Zhang, Y. & Lin, J. M. Qualitative and quantitative analysis of tumor cell metabolism via stable isotope labeling assisted microfluidic chip electrospray ionization mass spectrometry. *Anal Chem* **84**, 1695-1701, doi:10.1021/ac300003k (2012).
- 43 Gao, D., Li, H., Wang, N. & Lin, J. M. Evaluation of the absorption of methotrexate on cells and its cytotoxicity assay by using an integrated microfluidic device coupled to a mass spectrometer. *Anal Chem* **84**, 9230-9237, doi:10.1021/ac301966c (2012).
- 44 Gao, D., Liu, H., Lin, J. M., Wang, Y. & Jiang, Y. Characterization of drug permeability in Caco-2 monolayers by mass spectrometry on a membrane-based microfluidic device. *Lab Chip* **13**, 978-985, doi:10.1039/c2lc41215b (2013).
- 45 Mao, S., Zhang, J., Li, H. & Lin, J. M. Strategy for signaling molecule detection by using an integrated microfluidic device coupled with mass spectrometry to study cell-to-cell communication. *Anal Chem* **85**, 868-876, doi:10.1021/ac303164b (2013).

Supporting information

Microfluidic platforms

From its foundation as an independent discipline in the early '90s, LOC has matured and a few dominant platforms have emerged. These platforms can largely be categorized as compartmentalized and non-compartmentalized microfluidic techniques on the one hand and as continuous flow and static platforms on the other hand.

	Non-compartmentalized	Compartmentalized
Continuous flow	Laminar flow techniques; electro-osmotic flow	Droplet microfluidics
		Centrifugal microfluidics
Static liquid or stop flow	Biosensors, arrays, magnetic bead platforms; dielectrophoresis	Large Scale Integration (Quake valves); Electrowetting

Continuous flow techniques are among the earliest to be used in the field of LOC. These platforms typically exploit the laminar flow regime in low Reynolds number flows that are associated with microfluidic dimensions. Mixing typically occurs by diffusion. Surfaces or immobilized objects can be addressed in a spatially differentiated pattern of multiple reactants. Electro-osmosis is a frequently used phenomenon for inducing flow in channels. Typically, electro-osmotic actuation is combined with some type of separation of such as electrophoresis, ITP or gradient focusing.

Non-compartmentalized, static flow or stop flow platforms are primarily used in conjunction with biosensors including microarrays and next generation sequencing set-ups and immunoassays. Although these microfluidic structures are referred to as “flow cells” in reference to buffer and reagent flushing steps, the reaction steps typically occur under static liquid conditions. Also cell and molecular manipulation techniques are frequently executed under static

conditions making use of actuation techniques such as dielectrophoresis, magnetic bead actuation or acoustics.

Compartmentalized platforms can also be subdivided in continuous flow and static or stop flow platforms. Compartmentalization of droplet based microfluidics is achieved by having an emulsion of aqueous droplets in a non-miscible oil phase. As such, each droplet functions as a microreactor enabling droplet separation, merging, mixing, assaying and reacting. The continuous flow conditions under which thousands of droplets can be processed in series, makes this platform highly promising as a high throughput analysis platform.

Static compartmentalized platforms include Large Scale Integration (LSI) techniques and electrowetting platforms. Large scale integrations techniques make use of silicon rubber valves (also called Quake valves after its inventor Stephen Quake) out of polydimethylsiloxane (PDMS). The valves are used to compartmentalize and actuate samples and enable large scale integration leading to thousands of samples to be processed in parallel. Electrowetting platforms make use of droplets immersed in oil or air that are individually actuated and transported using electrostatic forces. Particular large scale integration is a highly successful platform that is used extensively in the academic world and yielded a range of commercial products.

A mixed model is represented by spinning disc microfluidic platforms (Lab-on-a-Disc) that enables both reactions under flow conditions and under static conditions, by making use of centrifugal and Coriolis forces for liquid transportation, centrifugation and separation.