



Universiteit  
Leiden  
The Netherlands

## **Closed-Loop ventilation using sidestream versus mainstream capnography for automated adjustments of minute ventilation: a randomized clinical trial in cardiac surgery patients**

Nijbroek, S.G.L.H.; Roozeman, J.P.; Ettayeb, S.; Rosenberg, N.M.; Meenen, D.M.P. van; Cherpanath, T.G.V.; ... ; Schultz, M.J.

### **Citation**

Nijbroek, S. G. L. H., Roozeman, J. P., Ettayeb, S., Rosenberg, N. M., Meenen, D. M. P. van, Cherpanath, T. G. V., ... Schultz, M. J. (2023). Closed-Loop ventilation using sidestream versus mainstream capnography for automated adjustments of minute ventilation: a randomized clinical trial in cardiac surgery patients. *Plos One*, 18(8). doi:10.1371/journal.pone.0289412

Version: Publisher's Version  
License: [Creative Commons CC BY 4.0 license](https://creativecommons.org/licenses/by/4.0/)  
Downloaded from: <https://hdl.handle.net/1887/3714824>

**Note:** To cite this publication please use the final published version (if applicable).

## RESEARCH ARTICLE

# Closed-Loop ventilation using sidestream versus mainstream capnography for automated adjustments of minute ventilation—A randomized clinical trial in cardiac surgery patients

Sunny G. L. H. Nijbroek<sup>1,2</sup>\*, Jan-Paul Roozeman<sup>1,2</sup>, Sarah Ettayeb<sup>1</sup>, Neeltje M. Rosenberg<sup>1,3</sup>, David M. P. van Meenen<sup>1,2</sup>, Thomas G. V. Cherpanath<sup>1</sup>, Wim K. Lagrand<sup>1</sup>, Robert Tepaske<sup>1</sup>, Robert J. M. Klautz<sup>4,5</sup>, Ary Serpa Neto<sup>1,6,7,8,9</sup>, Marcus J. Schultz<sup>1,10,11</sup>

**1** Department of Intensive Care, Amsterdam University Medical Centers, Location AMC, Amsterdam, The Netherlands, **2** Department of Anesthesiology, Amsterdam University Medical Centers, Location AMC, Amsterdam, The Netherlands, **3** Department of Internal Medicine, Spaarne Hospital, Haarlem, The Netherlands, **4** Department of Cardiothoracic Surgery, Amsterdam University Medical Centers, Location AMC, Amsterdam, The Netherlands, **5** Department of Cardiothoracic Surgery, Leiden University Medical Center, Leiden, The Netherlands, **6** Australian and New Zealand Intensive Care Research Centre (ANZIC-RC), School of Public Health and Preventive Medicine, Monash University, Melbourne, Australia, **7** Laboratory of Experimental Intensive Care and Anesthesiology (L-E-I-C-A), Amsterdam University Medical Centers, Location AMC, Amsterdam, The Netherlands, **8** Department of Critical Care, Austin Hospital, Melbourne Medical School, University of Melbourne, Melbourne, Australia, **9** Department of Critical Care Medicine, Hospital Israelita Albert Einstein, Sao Paulo, Brazil, **10** Nuffield Department of Medicine, University of Oxford, Oxford, United Kingdom, **11** Mahidol-Oxford Tropical Medicine Research Unit (MORU), Mahidol University, Bangkok, Thailand

\* These authors contributed equally to this work.

\* [s.g.nijbroek@amsterdamumc.nl](mailto:s.g.nijbroek@amsterdamumc.nl)



## OPEN ACCESS

**Citation:** Nijbroek SGLH, Roozeman J-P, Ettayeb S, Rosenberg NM, van Meenen DMP, Cherpanath TGV, et al. (2023) Closed-Loop ventilation using sidestream versus mainstream capnography for automated adjustments of minute ventilation—A randomized clinical trial in cardiac surgery patients. PLoS ONE 18(8): e0289412. <https://doi.org/10.1371/journal.pone.0289412>

**Editor:** Samuele Ceruti, Sant Anna Hospital: Clinica Sant'Anna, SWITZERLAND

**Received:** May 4, 2023

**Accepted:** July 18, 2023

**Published:** August 23, 2023

**Copyright:** © 2023 Nijbroek et al. This is an open access article distributed under the terms of the [Creative Commons Attribution License](https://creativecommons.org/licenses/by/4.0/), which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

**Data Availability Statement:** The anonymized study data has been uploaded to Figshare: DOI: [10.6084/m9.figshare.23825955](https://doi.org/10.6084/m9.figshare.23825955).

**Funding:** The author(s) received no specific funding for this work.

**Competing interests:** MJS was a part-time employee of Hamilton Medical AG, Bonaduz, Switzerland, where he was the team leader of the department of research and new technologies from

## Abstract

### Background

INTELLiVENT-Adaptive Support Ventilation (ASV) is a closed-loop ventilation mode that uses capnography to adjust tidal volume ( $V_T$ ) and respiratory rate according to a user-set end-tidal  $CO_2$  (et $CO_2$ ) target range. We compared sidestream versus mainstream capnography with this ventilation mode with respect to the quality of breathing in patients after cardiac surgery.

### Methods

Single-center, single-blinded, non-inferiority, randomized clinical trial in adult patients scheduled for elective cardiac surgery that were expected to receive at least two hours of postoperative ventilation in the ICU. Patients were randomized 1:1 to closed-loop ventilation with sidestream or mainstream capnography. Each breath was classified into a zone based on the measured  $V_T$ , maximum airway pressure, et $CO_2$  and pulse oximetry. The primary outcome was the proportion of breaths spent in a predefined 'optimal' zone of

January 2022 to January 2023. The other authors have no conflicts of interest.

ventilation during the first three hours of postoperative ventilation, with a non-inferiority margin for the difference in the proportions set at  $-20\%$ . Secondary endpoints included the proportion of breaths in predefined 'acceptable' and 'critical' zones of ventilation, and the proportion of breaths with hypoxemia.

## Results

Of 80 randomized subjects, 78 were included in the intention-to-treat analysis. We could not confirm the non-inferiority of closed-loop ventilation using sidestream with respect to the proportion of breaths in the 'optimal' zone (mean ratio 0.87 [0.77 to  $\infty$ ];  $P = 0.116$  for non-inferiority). The proportion of breaths with hypoxemia was higher in the sidestream capnography group versus the mainstream capnography group.

## Conclusions

We could not confirm that INTELLiVENT-ASV using sidestream capnography is non-inferior to INTELLiVENT-ASV using mainstream capnography with respect to the quality of breathing in subjects receiving postoperative ventilation after cardiac surgery.

## Trial registration

[NCT04599491](https://clinicaltrials.gov/ct2/show/study/NCT04599491) (clinicaltrials.gov).

## Introduction

INTELLiVENT-adaptive support ventilation (ASV) is a closed-loop ventilation mode that uses pressure-controlled or pressure support ventilation depending on patients' activity. Continuous pulse oximetry and capnography are used for adjustments of positive end-expiratory pressure (PEEP) and fraction of inspired oxygen ( $\text{FiO}_2$ ), and minute volume, respectively. Automatic adjustments are performed based on two equations, named 'Otis' and 'Mead' in order to reach the lowest work of breathing and force of breathing, respectively, according to user-set target ranges for end-tidal carbon dioxide ( $\text{etCO}_2$ ). Herein, the ventilator titrates the inspiratory pressure to reach an 'optimal' combination of tidal volume ( $V_T$ ) and respiratory rate (RR) [1–3]. This mode has been shown to be safe and effective with respect to the quality of breathing in various types of critically ill patients [4–6], and also in patients receiving ventilation after cardiac surgery [7–9].

With INTELLiVENT-ASV, either sidestream or mainstream capnography can be used, although these techniques have never been compared directly [10]. Sidestream capnography is mostly used during ventilation in the operating room, and it can be used in spontaneously breathing patients as well as pediatric patients where added weight and dead space in the airway circuit is undesirable [11–13]. The sidestream capnography technique causes less weight on the airway and the sensor is less fragile. One disadvantage of sidestream capnography, however, is the slight delay in readings due to sampling and transport of the air mixture to the sensor. Other disadvantages include poor readings due to accidental crushing or kinking of the sampling tube, and potential blockages by condensation from humidified sample gas, and airway secretions [14, 15]. In the adult ICU setting, mainstream capnography is most often used and widely available [16]. Mainstream capnography has the disadvantage that it increases dead space, and adds additional weight to the artificial airway, caused by the sensor block that is

usually placed close to the distal end of the endotracheal tube [15]. Additionally, this technique is costlier than sidestream capnography, and the sensor could easily be damaged during cleaning and storage [14, 15].

Thus far, clinical studies of INTELLiVENT-ASV only tested its safety and efficacy when using mainstream capnography. Sidestream capnography could serve as an attractive alternative for mainstream capnography, in certain settings and in several patient categories. The differences in the accuracies of the two techniques, however, could affect the performance of the closed-loop ventilation mode [17, 18]. Therefore, we performed a head-to-head comparison of these two alternate ways of capnography in a randomized clinical trial named 'INTELLiVENT-ASV using mainstream versus sidestream capnography in cardiac surgery patients' (INTELLiSTREAM). We hypothesized that closed-loop ventilation using sidestream capnography is non-inferior to closed-loop ventilation using mainstream capnography with respect to the quality of breathing.

## Methods

### Study design and oversight

INTELLiSTREAM was an investigator-initiated and investigator-sponsored, single-center, single-blinded, non-inferiority, randomized clinical trial comparing postoperative closed-loop ventilation using sidestream versus mainstream capnography. The study was performed at the Amsterdam University Medical Centers, location 'AMC', Amsterdam, the Netherlands. The trial was approved by the local Institutional Review Board (METC 2019\_222; Chair prof. dr. J.A. Swinkels; date of ethical approval march 6<sup>th</sup>, 2020) and registered at clinicaltrials.gov (study identifier NCT04599491). INTELLiSTREAM was performed in accordance to the principles of the Declaration of Helsinki, adhering to Good Clinical Practice guidelines including data monitoring. Written informed consent was obtained from all subjects prior to surgery.

### Study population

Subjects were eligible for participation if: (1) aged  $\geq 18$  years; (2) scheduled for elective cardiac surgery; and (3) expected to require at least two hours of ventilation after arrival in the ICU, e.g., patients scheduled for open valve surgery, aortic surgery or on-pump coronary artery bypass grafting. Exclusion criteria were previous inclusion in this study, and participation in another intervention that could influence ventilator settings and ventilation parameters. We also excluded subjects with confirmed or suspected pregnancy, and subjects that were expected to die in the first hours after surgery.

### Randomization

Subjects were randomized in a 1:1 ratio to receive closed-loop ventilation using sidestream or mainstream capnography. Randomization was performed by one of the study coordinators at the end of the surgical procedure shortly before transport to the ICU for postoperative care, using a web-based, password-protected program (<http://www.castoredc.com>), and permuted blocks with random block sizes. Subjects remained blinded to which capnography sensor was used during postoperative ventilation. Healthcare professionals could not be blinded because of the nature of the intervention. The investigator performing the statistical analysis, however, remained blinded for treatment allocation when analyzing the primary endpoint.

## Study procedures and data collection

In the ICU, subjects were typically cared for by one dedicated board-certified ICU nurse. Changes in treatment were implemented based on observations by the nurse, and according to the recommendations in the local guideline for postoperative care. Closed-loop ventilation was generally initiated within 10 minutes of ICU arrival, with automated adjustments of minute volume, PEEP and FiO<sub>2</sub> activated. Data was collected breath-by-breath until tracheal extubation, or up to a maximum of 6 hours, using a Memorybox data storage device (Hamilton Medical AG) attached directly to the ventilator. Extubation was performed according to criteria described in the local protocol. Follow-up was performed until 30 days after randomization. Further details regarding data collection and routine perioperative care can be found in the [S1 File](#). This study was performed in accordance with CONSORT guidelines for randomized controlled trials.

## Endpoints

Quality of breathing was scored using three predefined and previously used ventilation zones, named 'optimal', 'acceptable', and 'critical' ([Table 1](#)) [9]. For this, each breath was classified into one of these three zone based on the measured V<sub>T</sub>, maximum airway pressure (P<sub>max</sub>), etCO<sub>2</sub> and peripheral oxygen saturation by pulse oximetry (SpO<sub>2</sub>). We chose to use these definitions, to make the study results comparable to previous [9] and future studies on automated ventilation [19]. The primary endpoint was the *proportion of breaths* spent in the 'optimal zone' of ventilation during the first 3 hours of postoperative ventilation. In case of missing data, if all of the parameters were missing, the zone was considered missing. If parameters were missing, but one was available and in the critical zone, the zone was defined as critical. If parameters were missing, but one was available and not in the critical zone, the zone was defined as missing.

We had the following secondary endpoints: the proportion of breaths spent in the 'acceptable' and 'critical' zone in the first 3 hours of postoperative ventilation; the *proportion of time* spent in the predefined ventilation zones in the first 3 hours of postoperative ventilation; duration of weaning, defined as the time from cessation of sedatives until tracheal extubation; and

**Table 1. The predefined ventilation zones\*.**

	Critical Zone	Acceptable Zone	Optimal Zone
Tidal volume, ml/kg PBW	> 12 OR	8–12 AND/OR	≤ 8 AND
Maximum airway pressure, cm H <sub>2</sub> O	≥ 36 OR	31–36 AND/OR	≤ 30 AND
etCO <sub>2</sub> , mmHg	< 25 OR ≥ 51 OR	25–30 OR 46–51 AND/OR	30–46 AND
SpO <sub>2</sub> , %	< 85	≥ 98 OR 85–93	93–98 OR ≥ 93 if FiO <sub>2</sub> ≤ 40%
<b>Definitions</b>	if any parameters present: 'critical zone'	no parameters in 'critical zone', but not all parameters in 'optimal zone': 'acceptable zone'	if all parameters present: 'optimal zone'

\* Zones of ventilation adapted from: De Bie et al. [9]

These definitions have been used in previous studies on automated ventilation and they reflect the quality of breathing with respect to important ventilator variables, using generally accepted safety zones.

Abbreviations: etCO<sub>2</sub>: end-tidal carbon dioxide by mainstream capnography; FiO<sub>2</sub>: fraction of inspired oxygen; PBW, predicted body weight; SpO<sub>2</sub>: oxygen saturation by pulse oximetry

<https://doi.org/10.1371/journal.pone.0289412.t001>

total duration of postoperative ventilation, defined as the time from the start of ventilation in the ICU until tracheal extubation. We also collected the following endpoints: the proportion of failed extubations, defined as a reintubation within 48 hours after extubation, excluding subjects for a re-thoracotomy; incidence of postoperative pulmonary complications, defined as a collapsed composite of pneumonia, pneumothorax or severe atelectasis; length of stay in ICU and hospital; ICU readmission; mortality in ICU and at day 30; the incidence of hypoxemia, defined as the proportion of breaths with an  $\text{SpO}_2 < 85\%$ , but only when the  $\text{SpO}_2$  had a quality index of  $> 50\%$ , as well as ventilation parameters and the results from clinically-indicated arterial blood gas analyses.

### Sample size calculation

We estimated that a sample size of 72 subjects would provide 80% power, considering an expected proportion of breaths in the 'optimal' zone of ventilation with mainstream capnography of  $69 \pm 23\%$  [9], with a one-sided alpha level of 0.05 and a non-inferiority margin of 20%. This margin corresponds to 14% less breaths in the 'optimal' zone in the sidestream group compared to the mainstream group. Subjects that were extubated before 90 minutes of postoperative ventilation, were considered drop-outs and were replaced with new subjects. Thus, enrollment was continued until both study arms had at least 36 subjects with the minimum duration of 90 minutes of postoperative ventilation. The cutoff of 90 minutes was chosen to have sufficient time to observe the evolution of postoperative ventilation requirements, to increase the comparability of subjects, and to reduce the likelihood of clinical and statistical heterogeneity, as subjects rapidly awaking from anesthesia after surgery would likely have different respiratory needs.

### Statistical analysis

For the intention to treat analysis, we analyzed the recorded ventilation data according to the treatment that subjects actually received. Continuous variables are presented as medians with interquartile ranges (IQR), and categorical variables with numbers and proportions. Continuous data are presented as medians (quartile 25% to quartile 75%), regardless of distribution, for consistency and to enhance readability.

The proportion of breaths in the 'optimal', 'acceptable' and 'critical' zones is summarized per subject according to the following equation:


$$\text{proportion of breaths in zone} = (\text{number of breaths in zone} / \text{total number of breaths}) \text{ (Eq1)}$$

Data for the primary outcome are presented as median (quartile 25% to quartile 75%) and mean  $\pm$  standard deviation, and compared as a mean ratio (Eq 2) tested for non-inferiority considering a margin of 20%, and presented with a one-sided 95% confidence interval (95%-CI):

$$\text{Mean Ratio} = (\text{Mean proportion of breaths in zone for Sidestream} / \text{Mean proportion of breaths in zone for Mainstream}) \text{ (Eq2)}$$

A one-sided *P* value for non-inferiority was calculated. Non-inferiority was established if the lower boundary of the one-sided 95% confidence interval was higher than 0.80 (indicating 20% decrease in proportion of breaths in the optimal zone). If non-inferiority was confirmed, superiority for sidestream capnography was to be tested considering a 95% CI following hierarchical closed testing procedure.

All analysis for secondary endpoints tested for superiority and were two-sided. For secondary outcomes assessing the proportion of breaths and the incidence of hypoxemia, the

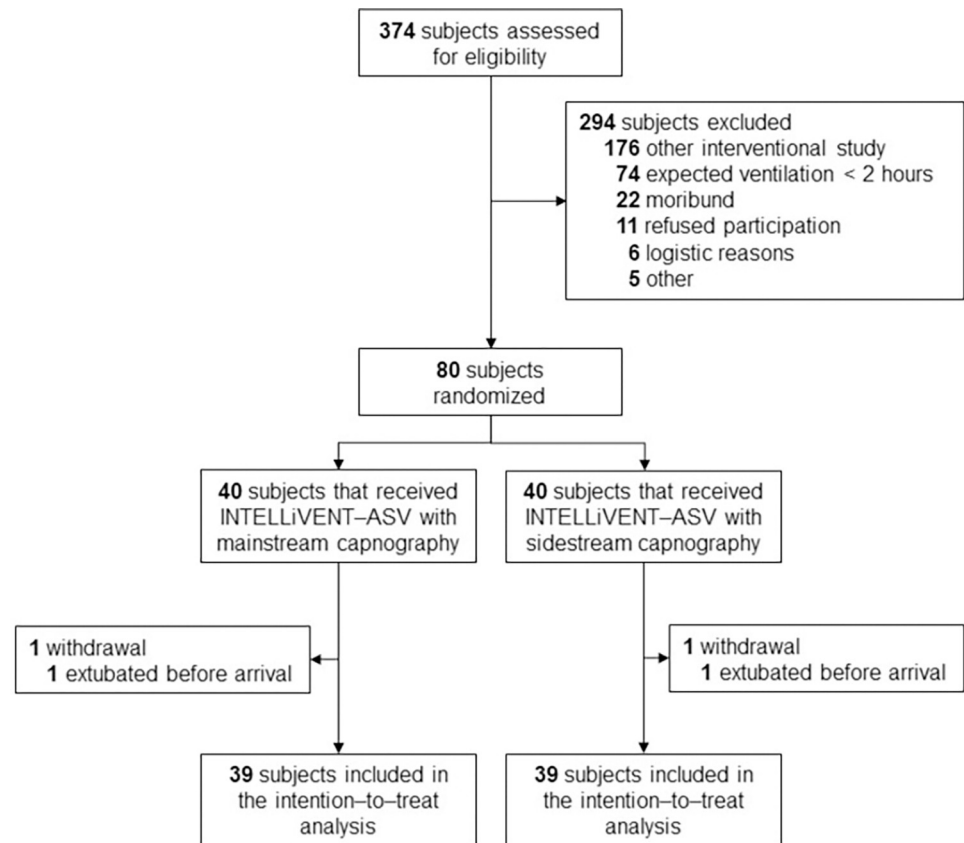

**Fig 1. CONSORT flow diagram.**

<https://doi.org/10.1371/journal.pone.0289412.g001>

denominator was the total number of breaths. The proportion of breaths in acceptable and critical zones, or with hypoxemia were analyzed using the same strategy as the primary outcome. For all other secondary endpoints, effect estimates were calculated using univariate logistic or linear regression, for binary and continuous endpoints respectively.

In creating the per protocol analysis, we excluded subjects who had one or more major protocol violations, i.e., not meeting minimum ventilation time requirement, or receiving ventilation with the capnography sensor that they were not assigned to.

Treatment effect on the primary outcome was analyzed according to following subgroups: 1) subjects who were successfully extubated before or after median postoperative ventilation duration; 2) subjects with shorter or longer than median intraoperative ventilation duration; and 3) subjects with  $\text{PaO}_2/\text{FiO}_2$  ratio below or above the median at admission in the ICU. The effect of subgroups was evaluated according to the interaction effects between each subgroup and the study arms following the primary analysis.

For the analyses of ventilation parameters over the first three hours of ventilation, all parameters were summarized as the mean of every 5 minutes until extubation or 180 minutes, whichever came first. Sidestream and mainstream groups were compared using mixed-effect longitudinal models with the subjects as random effect, the variable of interest as the dependent variable and the time of measurement, randomization group and an interaction of time and randomization group as fixed effects.

The effects of the intervention on the duration of weaning, and the time until ICU and hospital discharge were assessed using Kaplan-Meier survival curves and a log rank test to

calculate a two-sided  $P$  value for hypothesis testing. Survival time was calculated from the time of randomization until the time of the outcome. Patients who died during follow-up were censored for Kaplan-Meier estimates. Lastly, for quality checking we plotted a comparison between sensors of capnography measurements every 10 minutes for the first three hours of postoperative ventilation.

All analyses were performed using R statistical software (version 4.1.0, R Core Team, 2016, Vienna, Austria), and a  $P < 0.05$  was considered statistically significant.

## Results

### Cohort characteristics

Between June 2020 and May 2022, 374 subjects were screened for eligibility (Fig 1). A total of 294 subjects were excluded, mostly due to participation in another interventional study, or the expectation that postoperative ventilation would last less than two hours. Two subjects withdrew from the study because they were extubated directly upon arrival at the ICU, and thus did not receive postoperative ventilation with the assigned closed-loop ventilation mode. Of the remaining 78 subjects, the surgical and baseline characteristics are shown in Table 2. Most of the subjects were male, and the majority underwent either coronary arterial bypass graft surgery or aortic valve surgery. The most common non-cardiac comorbidities were hypertension and diabetes mellitus.

### Ventilator parameters

In the first hour after randomization, median RR and  $\text{FiO}_2$  were higher, and median  $V_T$  was lower in the sidestream capnography group; thereafter, there were no differences between the two groups (S1–S6 Figs). Compared to sidestream capnography,  $\text{etCO}_2$  measurements during mainstream capnography were higher at all time points (S7 Fig).

### Primary outcome

During the first three hours of postoperative ventilation, the median *proportion of breaths* in the optimal zone of ventilation was 0.77 [IQR, 0.51–0.91] and 0.84 [IQR, 0.67–0.91] in the sidestream capnography and mainstream capnography groups, respectively, (mean ratio 0.87 (one-sided 95% CI 0.77– $\infty$ );  $P = 0.116$  for non-inferiority), crossing the pre-defined non-inferiority margin of 0.80 (Fig 2 and Table 3). The per protocol analysis did not change this finding (S1 Table).

### Secondary outcomes

No differences were found between groups for the median *proportion of breaths* spent in the acceptable and critical zones of ventilation. The median *proportion of time* spent in the optimal, acceptable or critical zones of ventilation was also not different between groups. There was a statistically significant difference in the proportion of breaths with hypoxemia between the two groups (0.00 vs. 0.00, mean ratio 4.59 [1.23–20.42],  $P = 0.037$ ). There were no differences in the clinical endpoints (Table 2 and S8 Fig).

### Subgroup analysis

The effect of the used capnography technique on the median proportion of breaths in the optimal zone of ventilation was consistent across the three predefined subgroups (S9 Fig).



Table 2. Baseline characteristics.

	Sidestream capnography (N = 39)	Mainstream capnography (N = 39)
Age, years	65.0 [60.0–70.5]	68.0 [63.0–73.5]
Male gender, %	30/39 (76.9)	26/39 (66.7)
PBW, kg	70.6 [64.7–78.3]	72.4 [63.3–78.3]
BMI, kg/m <sup>2</sup>	26.0 [24.1–29.0]	25.9 [22.6–29.6]
SAPS II score available	39/39 (100.0)	36/39 (92.3)
Median SAPS II score	27.0 [23.5–31.5]	26.0 [23.0–29.0]
EuroSCORE II available	38/39 (97.4)	38/39 (97.4)
Median EuroSCORE II score	1.5 [1.0–2.4]	1.7 [1.0–2.0]
APACHE IV score available	39/39 (100.0)	36/39 (92.3)
Median APACHE IV score	38.0 [33.0–46.0]	40.0 [30.8–44.3]
Smoking status, %		
Never	12/39 (30.8)	14/39 (35.9)
Former (cessation >3 months ago)	19/39 (48.7)	21/39 (53.8)
Current	8/39 (20.5)	4/39 (10.3)
Alcohol use, %		
Never	13/39 (33.3)	11/39 (28.2)
Occasional	16/39 (41.0)	16/39 (41.0)
Frequent	10/39 (25.6)	11/39 (28.2)
Yes, but frequency unclear	0/39 (0.0)	1/39 (2.6)
COPD, %	1/39 (2.6)	1/39 (2.6)
Asthma, %	1/39 (2.6)	1/39 (2.6)
Diabetes Mellitus, %	8/39 (22.2)	7/39 (17.9)
Diet only	1/39 (2.6)	0/39 (0.0)
Oral medication	5/39 (12.8)	3/39 (7.7)
Insulin	2/39 (5.1)	4/39 (10.3)
Hypertension, %	21/39 (53.8)	20/39 (51.3)
OSAS, %	3/39 (7.7)	1/39 (2.6)
Chronic Kidney Injury, %	2/39 (5.2)	0/39 (0.0)
Cerebral Vascular Incident, %	1/39 (2.6)	2/39 (5.1)
Peripheral artery disease, %	3/39 (7.7)	4/39 (10.3)
NYHA classification, %		
Not applicable	10/39 (25.6)	5/39 (12.8)
I	9/39 (23.1)	10/39 (25.6)
II	9/39 (23.1)	13/39 (33.3)
III	9/39 (23.1)	9/39 (23.1)
IV	2/39 (5.1)	2/39 (5.1)
Left Ventricle Ejection Fraction	0.5 [0.5–0.6]	0.5 [0.4–0.5]
Left Ventricle Function, categories		
Reduced (<40%)	3/39 (7.7)	3/39 (7.7)
Mid-range (40–50%)	6/39 (15.4)	10/39 (25.6)
Normal (>50%)	30/39 (76.9)	26/39 (66.7)
Right Ventricle function, categories		
Moderate	2/39 (5.1)	0/39 (0.0)
Good	37/39 (94.9)	39/39 (100.0)
Pulmonary hypertension	1/39 (2.6)	4/39 (10.3)
Atrial Fibrillation	10/39 (25.6)	12/39 (30.8)
Aortic Valve Disease		

(Continued)

Table 2. (Continued)

	Sidestream capnography (N = 39)	Mainstream capnography (N = 39)
None	24/39 (61.5)	18/39 (46.2)
Moderate Insufficiency	9/39 (23.1)	8/39 (20.5)
Severe Insufficiency	4/39 (10.3)	3/39 (7.7)
Moderate Stenosis	1/39 (2.6)	2/39 (5.1)
Severe Stenosis	7/39 (17.9)	14/39 (35.9)
Mitral Valve Disease		
None	23/39 (59.0)	18/39 (46.2)
Moderate Insufficiency	9/39 (23.1)	14/39 (35.9)
Severe Insufficiency	6/39 (15.4)	6/39 (15.4)
Moderate Stenosis	0/39 (0.0)	2/39 (5.1)
Severe Stenosis	1/39 (2.6)	0/39 (0.0)
Tricuspid Valve Disease		
None	31/39 (79.5)	29/39 (74.4)
Moderate Insufficiency	8/39 (20.5)	10/39 (25.6)
Severe Insufficiency	1/39 (2.6)	0/39 (0.0)
Moderate Stenosis	0/39 (0.0)	0/39 (0.0)
Severe Stenosis	0/39 (0.0)	0/39 (0.0)
Perioperative characteristics		
Type of Surgery, %		
CABG	18/39 (46.2)	15/39 (38.5)
Aortic Root	7/39 (17.9)	7/37 (17.9)
Aortic Arch	1/39 (2.6)	3/39 (7.7)
Aortic Valve	13/39 (33.3)	21/39 (53.8)
Mitral Valve	6/39 (15.4)	7/39 (17.9)
Tricuspid Valve	4/39 (10.3)	1/39 (2.6)
Pacemaker	0/39 (0.0)	0/39 (0.0)
Duration of anesthesia, minutes	325.0 [286.3–386.5]	322.0 [278.0–351.0]
Duration of extracorporeal circulation, minutes	122.0 [101.0–162.5]	131.0 [104.0–157.0]
Duration of aortic occlusion, minutes	93.0 [62.5–124.0]	99.0 [61.5–117.0]
First postop CK-MB, ng/mL	26.4 [17.4–42.0]	23.4 [18.6–39.9]


Data are presented as numbers (percentage) or medians [1<sup>st</sup> quartile–3<sup>rd</sup> quartile]. For consistency and to enhance readability, we present all our continuous data using the median with interquartile ranges.

Abbreviations: APACHE IV, Acute Physiology and Chronic Health Evaluation Score; BMI, Body Mass Index; CABG, Coronary Artery Bypass Graft; CK-MB, Creatine Kinase MB Isoenzyme; COPD, Chronic Obstructive Pulmonary Disease; OSA, Obstructive Sleep Apnea; PBW, Predicted Bodyweight; NYHA, New York Heart Association; SAPS II, Simplified Acute Physiology Score

<https://doi.org/10.1371/journal.pone.0289412.t002>

## Discussion

In this investigator-initiated, single-center, randomized clinical trial we compared the quality of breathing during postoperative ventilation between closed-loop ventilation using sidestream capnography versus mainstream capnography in elective cardiac surgery subjects. We could not confirm the non-inferiority of INTELLiVENT-ASV using sidestream capnography with respect to the proportion of breaths in the predefined optimal zone of ventilation. There was a statistically significant difference in the incidence of breaths with hypoxemia between the groups—this difference disappeared within the first hour of postoperative ventilation. There were no differences in the other endpoints.

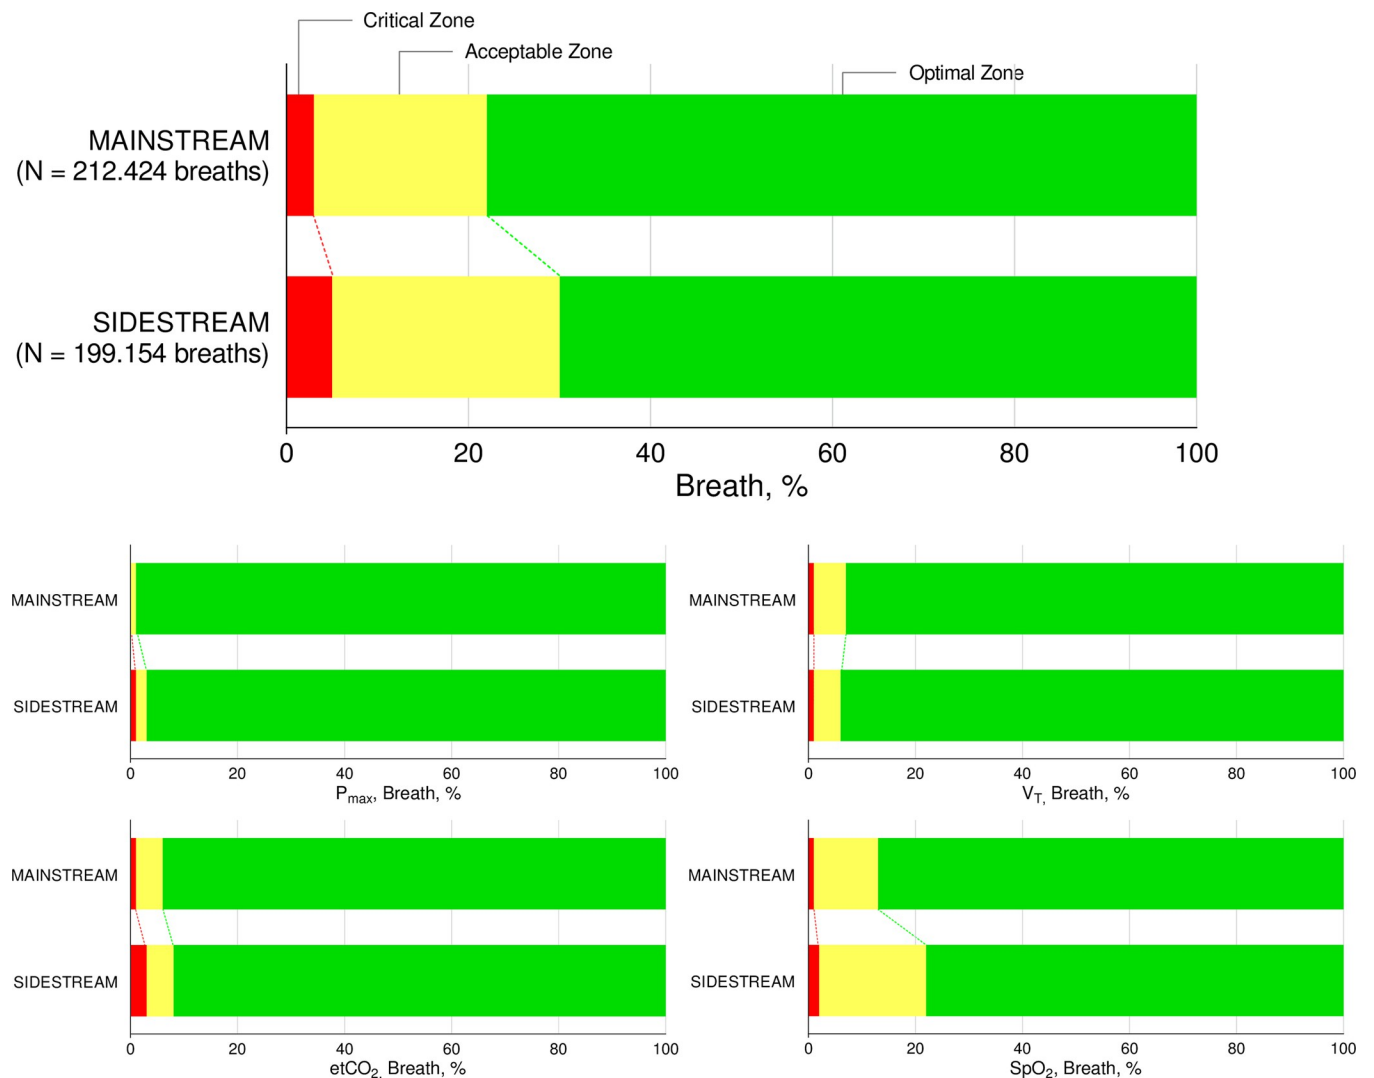

**Fig 2. Proportions of breaths in the predefined zones of ventilation.**

<https://doi.org/10.1371/journal.pone.0289412.g002>

This study has several strengths. The trial was performed in a setting where nurses and doctors had extensive experience with the tested closed-loop ventilation mode. The study protocol was straightforward and easy to follow. We used high density, i.e., breath-by-breath ventilator data that was collected directly from the ventilator for the main endpoints. This allowed for an accurate and highly granular comparison of the quality of breathing between the two study groups. The endpoints were predefined and used before [9]. The amount of missing data was low and follow-up was complete. The results of the per-protocol analysis were consistent with the intention-to-treat analysis, adding to the robustness of our findings. Lastly, our study was performed according to recent recommendations pertaining to the reporting of non-inferiority trials [20].

There are several possible explanations for why there were less breaths in the optimal zone in the sidestream group. Sampling delay is a well-known caveat of sidestream capnography, since gas sampling and subsequent transport from the main ventilation circuit to the sensor is required [21]. This is in obvious contrast to mainstream capnography, where the gas mixture

**Table 3. Primary endpoint and secondary endpoints.**

	Sidestream (N = 39)	Mainstream (N = 39)	Mean Ratio (95%- CI)	Absolute Mean Difference (95%-CI)	Odds Ratio (95%- CI)	P
<b>Primary endpoint</b>						
Proportion of breaths in optimal zone			0.87 (0.77 to ∞)			0.116*
Median [IQR]	0.77 [0.51–0.91]	0.84 [0.67–0.91]				
Mean ± standard deviation	0.69 ± 0.26	0.79 ± 0.16				
<b>Secondary endpoints</b>						
Proportion of breaths in acceptable zone						
Median	0.13 [0.08–0.39]	0.15 [0.08–0.27]	1.31 (0.87 to 1.91)			0.181
Mean	0.25 ± 0.23	0.19 ± 0.14				
Proportion of breaths in critical zone						
Median	0.02 [0.01–0.06]	0.01 [0.00–0.03]	2.69 (0.87 to 7.44)			0.072
Mean	0.07 ± 0.14	0.03 ± 0.04				
Proportion of time spent in optimal zone						
Median	0.86 [0.50–0.91]	0.85 [0.71–0.91]				
Mean	0.70 ± 0.24	0.79 ± 0.16		-0.09 (-0.18 to 0.00)		0.057
Proportion of time spent in acceptable zone						
Median	0.13 [0.08–0.38]	0.14 [0.08–0.28]				
Mean	0.24 ± 0.21	0.19 ± 0.14		0.05 (-0.03 to 0.14)		0.203
Proportion of time spent in critical zone						
Median	0.02 [0.01–0.05]	0.01 [0.00–0.03]				
Mean	0.06 ± 0.12	0.02 ± 0.04		0.04 (-0.01 to 0.09)		0.101
Proportion of breaths with SpO <sub>2</sub> <85%						
Median	0.00 [0.00–0.00]	0.00 [0.00–0.00]	4.59 (1.23 to 20.42)			0.037
Mean	0.00 ± 0.01	0.00 ± 0.00				
Exact values	247 / 75.327	107 / 82.323				
Duration of postoperative ventilation, hours	4.5 [2.3–5.4]	4.2 [3.0–5.9]		-0.39 (-1.62 to 0.84)		0.532
Duration of weaning, hours	1.2 [0.7–2.5]	1.7 [0.9–3.4]		-0.19 (-0.94 to 0.56)		0.556
Reintubations, %	2 / 39 (5.1)	1 / 39 (2.6)			2.05 (0.19 to 45.31)	0.564
Failed extubations, %	1 / 39 (2.6)	0 / 39 (0.0)			-	1.000
Postoperative Pulmonary Complications, %	5 / 39 (12.8)	7 / 39 (17.9)			0.68 (0.18 to 2.32)	0.532
Atelectasis	2 / 39 (5.1)	0 / 39 (0.0)			-	0.474
Pneumonia	2 / 39 (5.1)	1 / 39 (2.6)			2.05 (0.19 to 45.31)	0.564
Pneumothorax	3 / 36 (7.7)	6 / 39 (15.4)			0.45 (0.09 to 1.88)	0.296
Length of stay in ICU, days	1.0 [1.0–1.0]	1.0 [1.0–1.0]		0.18 (-0.84 to 1.20)		0.728
Length of stay in hospital, days	7.5 [5.6–10.6]	7.6 [6.5–10.5]		1.63 (-1.16 to 4.42)		0.248
Mortality, %						
Mortality at day 30	2 / 39 (5.1)	1 / 39 (2.6)			2.05 (0.19 to 45.31)	0.564
ICU mortality	0 / 39 (0.0)	0 / 39 (0.0)			-	-

Data are presented as numbers (percentage) or medians [1st quartile–3rd quartile]. For consistency and to enhance readability, we present all our continuous data using the median with interquartile ranges.

\*P for non-inferiority

Abbreviations: CI, confidence interval; SpO<sub>2</sub>, peripheral oxygen saturation.

<https://doi.org/10.1371/journal.pone.0289412.t003>

is analyzed directly in the circuit. Previous studies in subjects during supine craniotomy and cardiac surgery in the operating room, during noninvasive ventilation in the ICU, and in spontaneously breathing subjects in the emergency room have shown more variable and less accurate  $\text{etCO}_2$  measurements with sidestream capnography [17, 18, 22, 23]. Similar findings come from studies in pediatric populations, especially during periods with higher respiratory rates [24, 25]. Possible reasons for a larger variation in  $\text{etCO}_2$  with sidestream capnography could be due to the addition of inspiratory fresh gas flow to the gas mixture during sampling, or due to variable sampling flow rates during inspiration and expiration due to alternating airway pressures with each breath cycle. These phenomena might also explain the consistently higher  $\text{etCO}_2$  measurements using mainstream capnography in our study, and limit the applicability of sidestream capnography in situations where accurate high-frequency sampling is critical for rapid adjustments in care. However, this may not apply to patients receiving simple postoperative ventilation for a relatively short period of time.

Interestingly, ventilation using sidestream capnography resulted in a higher median RR and a lower median  $V_T$ , early after start of postoperative ventilation. A transiently higher  $\text{FiO}_2$  was also seen in the first hour of ventilation. During closed-loop ventilation the computer automatically adjusts ventilation parameters breath-by-breath based on continuous capnography and pulse oximetry readings. It is conceivable that due to the increased variability in sidestream capnography, the ventilator could have corrected high  $\text{etCO}_2$  measurements by increasing respiratory rate, as the tested closed-loop ventilation mode tries to continue applying lung-protective ventilation using low tidal volumes. The higher RR, however, shortens the inspiratory time, and may even cause a certain level of intrinsic PEEP, and perhaps even some overdistension. The latter could also explain the early differences in oxygenation—it is possible that overdistension led to an increase in perfusion of the dependent lung parts that may have been atelectatic early after surgery, thereby increasing ventilation-perfusion mismatch.

Our study increases the understanding of how the tested closed-loop ventilation mode affects ventilator settings and ventilation parameters during postoperative ventilation. Thus far, only two studies directly compared the quality of breathing between closed-loop ventilation and conventional ventilation in postoperative cardiac surgery subjects [7, 9]. Both studies found closed-loop ventilation to be superior to conventional ventilation with regard to the quality of breathing, using slightly different criteria. In one of these studies, with closed-loop ventilation using mainstream capnography more than two-third of breaths were in the optimal zone of ventilation. We confirmed this finding in our study, in both the mainstream and the sidestream group. Indeed, one silent finding in our study was the large proportion of breaths in the optimal zone, also when using sidestream capnography. The time spent in the critical zone using mainstream capnography was comparable to results of the other study that used comparable definitions for the quality of breathing [7]. Furthermore, in that study conventional ventilation resulted in more time in the critical zone when compared to sidestream capnography in our study. Thus, even though we were not able to verify the non-inferiority of closed-loop ventilation using sidestream when compared to mainstream capnography, closed-loop ventilation using sidestream capnography remains an efficacious and attractive way of providing postoperative ventilation.

This study also has limitations. First, due to the nature of the intervention, caregivers and data collectors could not be blinded for treatment allocation. However, the statistical analysis was performed by an investigator blinded for treatment allocation. Second, this was a single-center trial in a tertiary hospital with extensive experience with closed-loop ventilation. Therefore, it is possible that our findings are not directly generalizable to settings with less experience or less resources. Third, our sample size was not powered to observe differences in secondary clinical endpoints, and all findings should be seen as exploratory. Fourth, as the

majority of patients were expected to be extubated within the first 3 hours after start of ventilation in the ICU, we restricted the analysis to the first 3 hours. If the quality of breathing is different at later time points, it could be the subject of a future investigation. Fifth, to increase comparability between patients and homogeneity of the study cohort we adhered to a predefined minimum required time period of postoperative ventilation in the ICU which allowed for an assessment without confounding by duration of ventilation, but this may result in an incomplete reflection of the clinical variability, and with that the quality of breathing with either capnography method. Lastly, as we studied a typical cohort of patients, i.e., one in which ventilation is simple and short-lasting, we cannot give recommendations for use in other patient groups—this applies in particular to patients who benefit from a strict tailoring of the arterial CO<sub>2</sub> level.

Based on the results of our study, closed-loop ventilation with sidestream capnography should not be preferred over closed-loop ventilation with mainstream capnography in settings where mainstream capnography is widely available, and in subjects wherein mainstream capnography has little or no disadvantages. However, the results of our study should also be interpreted in the context of the non-inferiority design. Moreover, although the non-inferiority of closed-loop ventilation with sidestream could not be established for the quality of breathing, it is uncertain whether this also translates into clinical endpoints.

## Conclusion

This study could not confirm that INTELLiVENT-ASV using sidestream capnography is non-inferior to INTELLiVENT-ASV using mainstream capnography with respect to the quality of breathing in subjects receiving postoperative ventilation after cardiac surgery.

## Supporting information

### **S1 Checklist. CONSORT checklist.**

(PDF)

### **S1 File. Supplementary methods.**

(DOCX)

### **S2 File. INTELLiSTREAM trial protocol.**

(PDF)

### **S3 File. INTELLiSTREAM statistical analysis plan.**

(DOCX)

### **S1 Table. Primary endpoint and secondary endpoints according to per protocol principle.**

(DOCX)

### **S1 Fig. Plot of tidal volume (V<sub>T</sub>), Respiratory Rate (RR) and minute ventilation according to capnography group over time.**

(TIF)

### **S2 Fig. Plot of FiO<sub>2</sub>, etCO<sub>2</sub> and SpO<sub>2</sub> according to capnography group over time.**

(TIF)

### **S3 Fig. Plot of PEEP, driving pressure (ΔP), plateau pressure (P<sub>plat</sub>), maximum airway pressure (P<sub>max</sub>) according to capnography group over time.**

(TIF)

**S4 Fig. Cumulative distribution plots of  $V_T$ , RR, MP at 30 minutes after ICU arrival.**  
(TIF)

**S5 Fig. Cumulative distribution plots of  $FiO_2$ ,  $etCO_2$  and  $SpO_2$  at 30 minutes after ICU arrival.**  
(TIF)

**S6 Fig. Cumulative distribution plots of PEEP,  $\Delta P$ , Pplat, Pmax at 30 minutes after ICU arrival.**  
(TIF)

**S7 Fig. Comparison of  $etCO_2$  measurements between capnography sensors for quality checking.**  
(TIF)

**S8 Fig. Kaplan Meijer plots for time to weaning, discharge from ICU and hospital.**  
(TIF)

**S9 Fig. Subgroup analyses on percentage of breaths in predefined optimal zone of ventilation.**  
(TIF)

## Author Contributions

**Conceptualization:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, David M. P. van Meenen, Thomas G. V. Cherpanath, Wim K. Lagrand, Robert Tepaske, Robert J. M. Klautz, Ary Serpa Neto, Marcus J. Schultz.

**Data curation:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, Sarah Ettayeb, Neeltje M. Rosenberg.

**Formal analysis:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, David M. P. van Meenen, Ary Serpa Neto, Marcus J. Schultz.

**Investigation:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, Neeltje M. Rosenberg, David M. P. van Meenen, Marcus J. Schultz.

**Methodology:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, David M. P. van Meenen, Robert Tepaske, Ary Serpa Neto, Marcus J. Schultz.

**Project administration:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, Sarah Ettayeb, Marcus J. Schultz.

**Resources:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, Robert Tepaske, Marcus J. Schultz.

**Software:** Sunny G. L. H. Nijbroek, David M. P. van Meenen.

**Supervision:** Ary Serpa Neto, Marcus J. Schultz.

**Validation:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, Sarah Ettayeb, Neeltje M. Rosenberg, David M. P. van Meenen, Ary Serpa Neto.

**Visualization:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, David M. P. van Meenen, Ary Serpa Neto, Marcus J. Schultz.

**Writing – original draft:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, Neeltje M. Rosenberg, David M. P. van Meenen, Thomas G. V. Cherpanath, Wim K. Lagrand, Robert Tepaske, Robert J. M. Klautz, Ary Serpa Neto, Marcus J. Schultz.

**Writing – review & editing:** Sunny G. L. H. Nijbroek, Jan-Paul Roozeman, Sarah Ettayeb, Neeltje M. Rosenberg, David M. P. van Meenen, Thomas G. V. Cherpanath, Wim K. Lagrand, Robert Tepaske, Robert J. M. Klautz, Ary Serpa Neto, Marcus J. Schultz.

## References

1. Botta M, Wenstedt EFE, Tsonas AM, Buiteman-Kruizinga LA, van Meenen DMP, Korsten HHM, et al. Effectiveness, safety and efficacy of INTELLiVENT-adaptive support ventilation, a closed-loop ventilation mode for use in ICU patients—a systematic review. *Expert Rev Respir Med*. 2021; 15(11):1403–13. Epub 2021/05/29. <https://doi.org/10.1080/17476348.2021.1933450> PMID: 34047244.
2. Otis AB, Fenn WO, Rahn H. Mechanics of breathing in man. *J Appl Physiol*. 1950; 2(11):592–607. Epub 1950/05/01. <https://doi.org/10.1152/jappl.1950.2.11.592> PMID: 15436363.
3. Mead J. The control of respiratory frequency. *Ann N Y Acad Sci*. 1963; 109:724–9. <https://doi.org/10.1111/j.1749-6632.1963.tb13500.x> PMID: 13934289.
4. Arnal JM, Wysocki M, Novotni D, Demory D, Lopez R, Donati S, et al. Safety and efficacy of a fully closed-loop control ventilation (IntelliVent-ASV®) in sedated ICU patients with acute respiratory failure: a prospective randomized crossover study. *Intensive Care Med*. 2012; 38(5):781–7. Epub 2012/03/31. <https://doi.org/10.1007/s00134-012-2548-6> PMID: 22460854.
5. Bialais E, Wittebole X, Vignaux L, Roeseler J, Wysocki M, Meyer J, et al. Closed-loop ventilation mode (IntelliVent®-ASV) in intensive care unit: a randomized trial. *Minerva Anesthesiol*. 2016; 82(6):657–68. Epub 2016/03/10. PMID: 26957117.
6. Clavieras N, Wysocki M, Coisel Y, Galia F, Conseil M, Chanques G, et al. Prospective randomized crossover study of a new closed-loop control system versus pressure support during weaning from mechanical ventilation. *Anesthesiology*. 2013; 119(3):631–41. Epub 2013/04/27. <https://doi.org/10.1097/ALN.0b013e3182952608> PMID: 23619172.
7. Lellouche F, Bouchard PA, Simard S, L'Her E, Wysocki M. Evaluation of fully automated ventilation: a randomized controlled study in post-cardiac surgery patients. *Intensive Care Med*. 2013; 39(3):463–71. Epub 2013/01/23. <https://doi.org/10.1007/s00134-012-2799-2> PMID: 23338569.
8. Beijers AJ, Roos AN, Bindels AJ. Fully automated closed-loop ventilation is safe and effective in post-cardiac surgery patients. *Intensive Care Med*. 2014; 40(5):752–3. Epub 2014/03/01. <https://doi.org/10.1007/s00134-014-3234-7> PMID: 24577110.
9. De Bie AJR, Neto AS, van Meenen DM, Bouwman AR, Roos AN, Lameijer JR, et al. Fully automated postoperative ventilation in cardiac surgery patients: a randomised clinical trial. *Br J Anaesth*. 2020; 125(5):739–49. Epub 2020/08/03. <https://doi.org/10.1016/j.bja.2020.06.037> PMID: 32739044.
10. Sensors and monitoring. [https://www.hamilton-medical.com/en\\_AU/Products/Consumables/Sensors-and-monitoring.html](https://www.hamilton-medical.com/en_AU/Products/Consumables/Sensors-and-monitoring.html): Hamilton Medical; 2023 [cited 2023 June 26].
11. Kugelman A, Zeiger-Aginsky D, Bader D, Shoris I, Riskin A. A novel method of distal end-tidal CO<sub>2</sub> capnography in intubated infants: comparison with arterial CO<sub>2</sub> and with proximal mainstream end-tidal CO<sub>2</sub>. *Pediatrics*. 2008; 122(6):e1219–24. Epub 2008/11/24. <https://doi.org/10.1542/peds.2008-1300> PMID: 19029196.
12. Williams E, Dassios T, Greenough A. Assessment of sidestream end-tidal capnography in ventilated infants on the neonatal unit. *Pediatr Pulmonol*. 2020; 55(6):1468–73. Epub 2020/03/18. <https://doi.org/10.1002/ppul.24738> PMID: 32187888.
13. Ortega R, Connor C, Kim S, Djang R, Patel K. Monitoring ventilation with capnography. *N Engl J Med*. 2012; 367(19):e27. <https://doi.org/10.1056/NEJMvcm1105237> PMID: 23134404.
14. Jaffe MB. Infrared measurement of carbon dioxide in the human breath: "breathe-through" devices from Tyndall to the present day. *Anesth Analg*. 2008; 107(3):890–904. Epub 2008/08/21. <https://doi.org/10.1213/ane.0b013e31817ee3b3> PMID: 18713902.
15. Block FE Jr., McDonald JS. Sidestream versus mainstream carbon dioxide analyzers. *J Clin Monit*. 1992; 8(2):139–41. Epub 1992/04/11. <https://doi.org/10.1007/BF01617434> PMID: 1583550.
16. Nassar BS, Schmidt GA. Capnography During Critical Illness. *Chest*. 2016; 149(2):576–85. Epub 2015/10/09. <https://doi.org/10.1378/chest.15-1369> PMID: 26447854.
17. Pekdemir M, Cinar O, Yilmaz S, Yaka E, Yuksel M. Disparity between mainstream and sidestream end-tidal carbon dioxide values and arterial carbon dioxide levels. *Respir Care*. 2013; 58(7):1152–6. Epub 2013/01/17. <https://doi.org/10.4187/respcare.02227> PMID: 23322889.
18. Chan KL, Chan MT, Gin T. Mainstream vs. sidestream capnometry for prediction of arterial carbon dioxide tension during supine craniotomy. *Anaesthesia*. 2003; 58(2):149–55. Epub 2003/02/04. <https://doi.org/10.1046/j.1365-2044.2003.03035.x> PMID: 12562411.



19. Botta M, Tsonas AM, Sinnige JS, De Bie AJR, Bindels A, Ball L, et al. Effect of Automated Closed-loop ventilation versus conventional Ventilation on duration and quality of ventilation in critically ill patients (ACTIVE)—study protocol of a randomized clinical trial. *Trials*. 2022; 23(1):348. Epub 20220423. <https://doi.org/10.1186/s13063-022-06286-w> PMID: 35461264; PubMed Central PMCID: PMC9034629.
20. Mauri L, D'Agostino RB, Sr. Noninferiority Trials. *N Engl J Med*. 2018; 378(3):304–5. <https://doi.org/10.1056/NEJMc1714668> PMID: 29342382.
21. Breen PH, Mazumdar B, Skinner SC. Capnometer transport delay: measurement and clinical implications. *Anesth Analg*. 1994; 78(3):584–6. <https://doi.org/10.1213/00000539-199403000-00027> PMID: 8109779.
22. Balogh AL, Petak F, Fodor GH, Tolnai J, Csorba Z, Babik B. Capnogram slope and ventilation dead space parameters: comparison of mainstream and sidestream techniques. *Br J Anaesth*. 2016; 117(1):109–17. <https://doi.org/10.1093/bja/aew127> PMID: 27317710; PubMed Central PMCID: PMC4913399.
23. Sakuraya M, Douno E, Iwata W, Takaba A, Hadama K, Kawamura N, et al. Accuracy evaluation of mainstream and sidestream end-tidal carbon dioxide monitoring during noninvasive ventilation: a randomized crossover trial (MASCAT-NIV trial). *J Intensive Care*. 2022; 10(1):17. Epub 20220318. <https://doi.org/10.1186/s40560-022-00603-w> PMID: 35303968; PubMed Central PMCID: PMC8932153.
24. Pascucci RC, Schena JA, Thompson JE. Comparison of a sidestream and mainstream capnometer in infants. *Crit Care Med*. 1989; 17(6):560–2. <https://doi.org/10.1097/00003246-198906000-00016> PMID: 2498039.
25. McEvedy BA, McLeod ME, Kirpalani H, Volgyesi GA, Lerman J. End-tidal carbon dioxide measurements in critically ill neonates: a comparison of side-stream and mainstream capnometers. *Can J Anaesth*. 1990; 37(3):322–6. <https://doi.org/10.1007/BF03005583> PMID: 2108814.