



Universiteit
Leiden

The Netherlands

Exploring the clinical applicability of quantitative near-infrared fluorescence imaging with indocyanine green: towards objective and standardized assessment of tissue perfusion

Tange, F.P.

Citation

Tange, F. P. (2026, September 15). *Exploring the clinical applicability of quantitative near-infrared fluorescence imaging with indocyanine green: towards objective and standardized assessment of tissue perfusion*. Retrieved from <https://hdl.handle.net/1887/4309589>

Version: Publisher's Version


License: [Licence agreement concerning inclusion of doctoral thesis in the Institutional Repository of the University of Leiden](#)

Downloaded from: <https://hdl.handle.net/1887/4309589>

Note: To cite this publication please use the final published version (if applicable).

Chapter 4



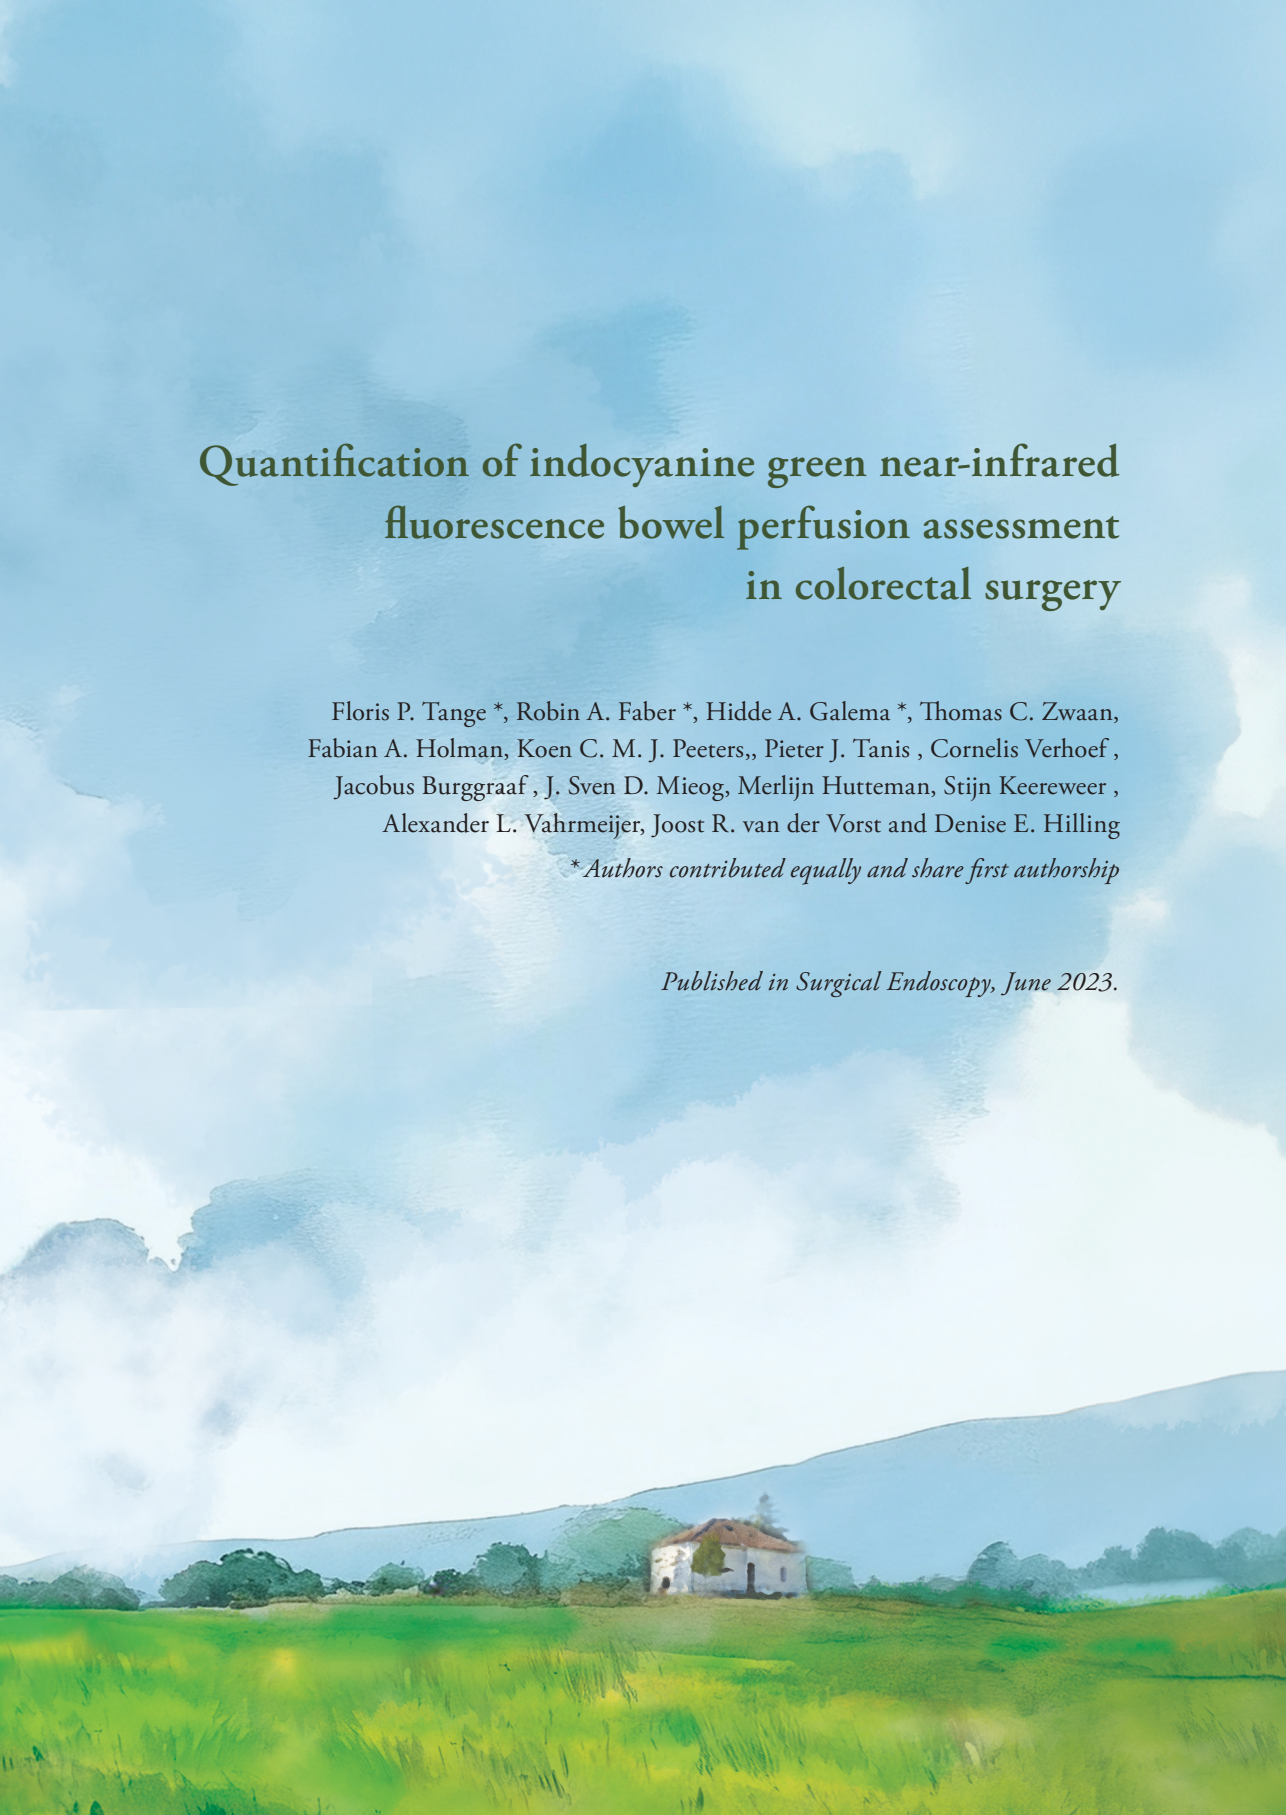

Quantification of indocyanine green near-infrared fluorescence bowel perfusion assessment in colorectal surgery

Floris P. Tange *, Robin A. Faber *, Hidde A. Galema *, Thomas C. Zwaan,
Fabian A. Holman, Koen C. M. J. Peeters,, Pieter J. Tanis , Cornelis Verhoef ,
Jacobus Burggraaf , J. Sven D. Mieog, Merlijn Hutteman, Stijn Keereweer ,
Alexander L. Vahrmeijer, Joost R. van der Vorst and Denise E. Hilling

** Authors contributed equally and share first authorship*

Published in Surgical Endoscopy, June 2023.

Abstract

Background

Indocyanine green near-infrared fluorescence bowel perfusion assessment has shown its potential benefit in preventing anastomotic leakage. However, the surgeon's subjective visual interpretation of the fluorescence signal limits the validity and reproducibility of the technique. Therefore, this study aimed to identify objective quantified bowel perfusion patterns in patients undergoing colorectal surgery using a standardized imaging protocol.

Method

A standardized fluorescence video was recorded. Postoperatively, the fluorescence videos were quantified by drawing contiguous region of interests (ROIs) on the bowel. For each ROI, a time-intensity curve was plotted from which perfusion parameters ($n = 10$) were derived and analyzed. Furthermore, the inter-observer agreement of the surgeon's subjective interpretation of the fluorescence signal was assessed.

Results

Twenty patients who underwent colorectal surgery were included in the study. Based on the quantified time-intensity curves, three different perfusion patterns were identified. Similar for both the ileum and colon, perfusion pattern 1 had a steep inflow that reached its peak fluorescence intensity rapidly, followed by a steep outflow. Perfusion pattern 2 had a relatively flat outflow slope immediately followed by its plateau phase. Perfusion pattern 3 only reached its peak fluorescence intensity after 3 min with a slow inflow gradient preceding it. The inter-observer agreement was poor-moderate (Intraclass Correlation Coefficient (ICC): 0.378, 95% CI 0.210–0.579).

Conclusion

This study showed that quantification of bowel perfusion is a feasible method to differentiate between different perfusion patterns. In addition, the poor-moderate inter-observer agreement of the subjective interpretation of the fluorescence signal between surgeons emphasizes the need for objective quantification.

Introduction

Anastomotic leakage (AL) is a serious postoperative complication in colorectal surgery with an incidence ranging from 1 to 20%.¹ It is associated with high morbidity and mortality, prolonged hospitalization, increased healthcare costs, and impaired oncological outcomes.^{2,3} The etiology of AL is multifactorial, in which compromised bowel perfusion is considered as a major contributing factor. Conventionally, bowel perfusion is assessed intraoperatively based on subjective clinical indicators, including tissue color, peristaltic movements, active bleeding from marginal arteries and palpable mesenteric arterial pulsations. Additional tests that may be used to assess the integrity of the anastomosis are the air leak test, intraoperative endoscopy and doughnut inspection.⁴ However, the surgeon's judgement of these clinical indicators was found to have low predictive value for AL, which indicates the need for more accurate intraoperative diagnostic tests.^{5,6}

Near-infrared (NIR) fluorescence imaging with indocyanine green (ICG) is a technique that enables real-time assessment of bowel perfusion. Several studies have shown its benefit to prevent AL.⁷ This is currently being validated in ongoing phase III randomized controlled trials, such as the AVOID trial⁸ (NCT04712032), IntAct trial⁹, and EssentialAL trial (jRCTs031180039), that should determine its clinical efficacy. However, the use of this technique is based on subjective visual interpretation of the fluorescence signal by the surgeon, which remains a limiting factor for the validity and reproducibility of these data in daily practice.^{10–13}

Quantitative evaluation of the fluorescence signal could increase the objectivity and accuracy of ICG NIR fluorescence bowel perfusion assessment. This method is based on the analysis of fluorescence intensity over time from which various inflow and outflow parameters can be derived. Some cohort studies have already investigated quantified bowel perfusion assessment using various generic quantification software.^{14–25} However, no consensus has been reached on which perfusion pattern and/or quantitative parameters can be considered to be sufficiently reliable to assess bowel perfusion.²⁶ This is partly due to the lack of a standardized imaging protocol, given the fact that intensity-based parameters are altered by camera-to-target distance, angle of camera-to-target tissue, type of imaging system and its settings.²⁷

This prospective cohort study aimed to identify quantified bowel perfusion patterns in patients undergoing colorectal surgery using a standardized imaging protocol. In addition, the inter-observer agreement of the surgeon's subjective interpretation of the fluorescence signal was assessed.

Methods

Study design and population

This prospective, dual center, exploratory study was conducted at the Leiden University Medical Center (LUMC) and Erasmus MC Cancer institute (EMC), according to the declaration of Helsinki (10th version, Fortaleza, 2013). Twenty patients with colorectal cancer who underwent ICG NIR fluorescence-guided colorectal resection with a primary anastomosis were included in the study. Medical ethical approval from the ethic committee Leiden-Den Haag-Delft was obtained (MEC-2021-0876). Informed consent was given by all patients.

Surgical procedure

A standardized imaging protocol was used to obtain fluorescence videos for quantification of the fluorescence signal. Fluorescence videos were recorded using the Quest Spectrum 2.0 camera system (Quest Medical Imaging, Middenmeer, the Netherlands). ICG NIR fluorescence bowel perfusion assessment was performed extracorporeally in all patients regardless the surgical approach chosen (i.e., open or minimally invasive surgery). In patients undergoing minimally invasive surgery (i.e., laparoscopic or robotic), the ileum and/or afferent/efferent colon was extracted extracorporeally through a Pfannenstiel incision. Before extracorporeal ICG NIR fluorescence bowel perfusion assessment, the camera was fixed in the camera arm and positioned 30 cm above the target tissue at an angle of 90 degrees. Standardized camera settings (GAIN: color 3.5 dB, ICG-fluor 20.0 dB; EXPOSURE: color 11.0 ms, ICG-fluor 50.0 ms) were maintained. After dissection of the vascular branch and prior to bowel transection, all patients received 5 mg ICG (2.5 mg/ml, Verdye, Diagnostic Green, Aschheim, Germany) intravenously followed by 10 mL saline flush according to standard care. Surgeons were allowed to change the surgical plan intraoperatively by performing an additional bowel resection based on their subjective interpretation of the fluorescence signal. Immediately after administration, a fluorescence video was recorded for 5 min. On each fluorescence video, the resection line was marked by the surgeon.

Quantitative analyses

The Quest Research Framework (Quest Medical Imaging, Middenmeer, the Netherlands) was used for quantification of the fluorescence videos. Postoperatively, contiguous region of interests (ROIs; approximately of 1 cm length) from proximal to distal of the resection line were drawn on the ileum or afferent/efferent colon, depending on the surgical procedure performed (Fig. 1). An example of a standardized fluorescence measurement is displayed in supplementary Video 1. The fluorescence signal as shown in Video 1 was quantified from multiple ROI's into corresponding time-intensity curves as illustrated in Fig. 1.

For each ROI, absolute (i.e., fluorescence intensity over time) and normalized (i.e., fluorescence intensity as a percentual change overtime by setting the maximum fluorescence intensity at 100 percent to minimize the influences of patient and camera-related factors²⁸) time-intensity curves were plotted from which 5 inflow and 5 outflow parameters were derived. These time-intensity curves were analyzed separately for the ileum and colon. The inflow parameters included the maximum fluorescence intensity (Imax), maximum inflow slope (Ingress slope), mean slope from baseline to maximum fluorescence intensity (Ingress rate), maximum inflow slope in percentage per second (Normalized slope), and time to maximum intensity (Tmax); the outflow parameters included the maximum outflow slope (Egress slope), area under the curve in percentage after 30, 60, 120, and 180 s from Tmax (AUC30, AUC60, AUC120, AUC180).

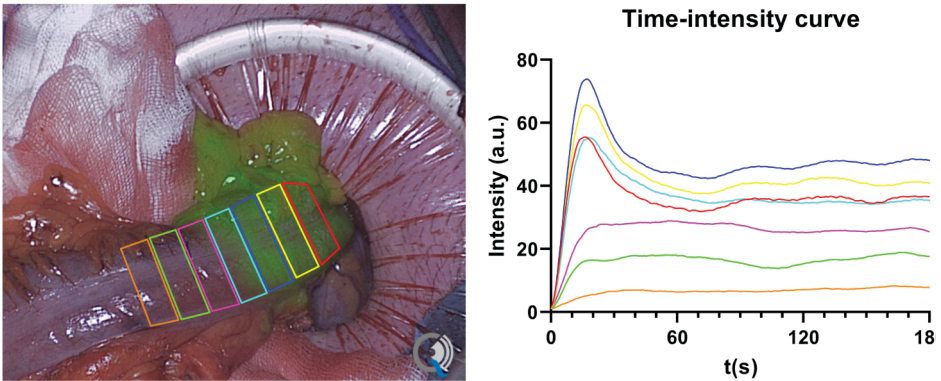


Figure. 1 Quantification of a standardized fluorescence video using the Quest Research Framework quantification tool. Contiguous region of interests (ROIs) were drawn from proximal to distal of the resection line (located at the dark blue ROI) on the afferent colon. For each ROI, an absolute time-intensity curve was plotted. The color of each time-intensity curve corresponds to the color of the ROI

Outcomes

The primary outcome of this study was to identify quantified bowel perfusion patterns in patients undergoing colorectal surgery by analyzing the time-intensity curves plotted from each ROI and its derived inflow and outflow perfusion parameters. The secondary outcomes were to assess the inter-observer agreement of the surgeon's subjective interpretation of the fluorescence signal and AIs after 90 days (i.e., early and late AI). The colorectal surgeons (FH, KP, DH, AB, GF, PT, CV) all experienced with fluorescence-guided surgery, were individually asked to mark the intended resection line on all 20 fluorescence videos, based on their subjective interpretation of the fluorescence signal.

The distance between the markers (i.e., intended resection lines) on each fluorescence video was measured with ImageJ (National Institutes of Health, USA), in which the most proximal marker was used as the baseline measurement according to the previously published method of Hardy et al.^{12, 13} AL was defined as AL that required active therapeutic intervention but manageable without reoperation (Grade B) or AL that requires reoperation (Grade C), according to the definition of the International Study Group of Rectal Cancer.^{29, 30} To associate the quantified perfusion patterns with the occurrence of AL, the time-intensity curves plotted from the ROIs of the anastomosis were analyzed.

The time-intensity curves of the anastomosis from both the afferent ileum or colon and the efferent colon were analyzed when both could be imaged extracorporeally. If not, only the time-intensity curves of the afferent ileum or colon were analyzed.

Statistical analyses

Patient characteristics were described using summary statistics. The distribution of all variables was assessed using histograms and verified with the Shapiro–Wilk test. Normally distributed variables were reported as means and standard deviation (SD) and skewed continuous variables were reported as medians and range. The inflow and out-flow parameters from different perfusion patterns were compared using the One-way ANOVA or Kruskal Wallis test, depending on the distribution. The inter-observer agreement of the surgeon's subjective interpretation of the fluorescence signal was assessed by calculating the intra-class correlation coefficient (ICC) according to a two-way mixed model, consistency type, single measurement method. An ICC < 0.50 indicated “poor agreement”, ICC ≥ 0.50 up to 0.75 indicated “moderate agreement”, ICC > 0.75 up to 0.90 indicated “good agreement”, and ICC > 0.90 indicated “excellent agreement”. All statistical analyses were performed using SPSS Version 25.0. The statistical outcomes were considered significant if the *p* value was < 0.05.

Results

Patient characteristics

Twenty patients (13 males; 7 females) with a median age of 63 years (range 46–83) were included in the analyses. Of these patients, 7 (35%) underwent a right-sided resection (i.e., ileocecal resection, right hemicolectomy or subtotal colectomy) and 13 (65%) patients underwent a left-sided resection (i.e., left hemicolectomy, sigmoid resection or low anterior resection). The majority (85%) of patients underwent surgery for a malignant tumor. Two (10%) patients received neo-adjuvant radiotherapy prior to surgical resection. A minimally invasive approach (i.e., laparoscopic or robotic) was performed in most patients (80%). The median in-hospital stay was 5 days (range 3–90).

In total, 2 patients died during hospitalization of which 1 died due to an acute coagulation disorder and 1 patient died from an acute myocardial infarction. A detailed overview of all patient characteristics is shown in Table 1.

Table 1. Patient characteristics

	TOTAL (n=20)
Age, median (range)	63 (46 – 83)
Male, n (%)	13 (65%)
BMI ^a , n (%)	
<30	14 (70%)
≥30	6 (30%)
ASA-score, n (%)	
1	1 (5%)
2	14 (70%)
3	5 (25%)
Smoking, n (%)	
Current	4 (20%)
Former	6 (30%)
Never	7 (35%)
Neoplasm, n (%)	
Benign	3 (15%)
Malignant	17 (85%)
Neo-adjuvant radiotherapy, n (%)	2 (10%)
Type of surgery, n (%)	
Right-sided resection ^b	7 (35%)
Left-sided resection ^c	13 (65%)
Surgical approach, n (%)	
Open	4 (20%)
Laparoscopic	11 (55%)
Robotic	5 (25%)
Type of anastomosis, n (%)	
Side-to-side isoperistaltic	4 (20%)
Side-to-side antiperistaltic	4 (20%)
Side-to-end	10 (50%)
End-to-side	0 (0%)
End-to-end	1 (5%)
Anastomosis technique, n (%)	
Handsewn	3 (15%)
Stapled	16 (80%)
Hospitalization in days, median (range)	5 (3 – 90)
Anastomotic leakage, n (%)	4 (20%)
Mortality, n (%)	2 (10%)

^a Body Mass Index (weight per kilogram/length²)

^b Included ileocecal resection, right hemicolectomy, and subtotal colectomy.

^c Included left hemicolectomy, sigmoid resection, and low anterior resection

Perfusion patterns

A total of 218 ROIs were drawn on the ileum or afferent/ efferent colon, with a mean number of 11 ± 3.8 ROIs per patient. From these ROIs, 35 (16%) time-intensity curves of the ileum and 183 (84%) time-intensity curves of the colon were plotted and analyzed.

Based on qualitative assessment of the quantified time-intensity curves, three different perfusion patterns were identified. Similar for both the ileum and colon, perfusion pattern 1 was characterized by a steep inflow slope (Ingress slope) that reached its peak fluorescence intensity (Tmax) rapidly, followed by a steep outflow slope (Egress slope). In contrast, perfusion pattern 2 had a relatively flat outflow slope immediately followed by its plateau phase. Perfusion pattern 3 only reached its peak fluorescence intensity after 3 min with a slow inflow gradient preceding it.

Cut-off points were determined for each perfusion pattern based on the quantified perfusion parameters. For the ileum, the time-intensity curves were distributed among the three different perfusion patterns using the following cut-off values; pattern 1: Tmax < 70 and Egress slope < - 2.5; pattern 2: Tmax < 70 and Egress slope $\geq$ - 2.5; pattern 3: Tmax $\geq$ 70.

The time-intensity curves of the colon were distributed using cut-off values such as pattern 1: Tmax < 70 and Egress slope < - 1; pattern 2: Tmax < 70 and Egress slope $\geq$ - 1; pattern 3: Tmax $\geq$ 70. The mean normalized time-intensity curve with standard deviation of each perfusion pattern for both the ileum and colon are shown in Fig. 2.

The mean quantified perfusion parameters of each perfusion pattern were compared for both the ileum and colon. The Imax, Ingress slope, Ingress rate, Normalized slope, Tmax, and Egress slope of the ileum differed significantly between the three perfusion patterns. The AUC30, 60, 120 and 180 did not differ significantly. The perfusion parameters of the colon were all significantly different between the three perfusion patterns as shown in Table 2.

Subjective interpretation of ICG NIR fluorescence imaging

All ($n = 20$) ICG NIR fluorescence imaging videos were independently assessed by 7 colorectal surgeons. The inter-observer agreement of the intended resection lines determined by the surgeons based on their subjective interpretation of the fluorescence signal was poor—moderate, with an ICC of 0.378 (95% CI 0.210–0.579). The median distance between the most proximal marker (i.e., baseline) and the most distal marker on the afferent and/or efferent ileum or colon was 1.122 cm (range 0.071–3.861). An overview of the distances (in centimeter) between the markers (i.e., intended resection lines) per fluorescence video are demonstrated in an ICC dot plot in Fig. 3.

The surgical plan has been changed in 4 (20%) patients by performing an additional bowel resection based on the intraoperative subjective interpretation of the fluorescence signal by the surgeon (Fig. 4). In 1 patient, perfusion pattern 2 was observed at the location of the intended anastomosis. After performing additional bowel resection, perfusion pattern 1 was observed.

Perfusion pattern 3 was observed in the other 3 patients at the location of the intended anastomosis and after additional bowel resection, perfusion pattern 2 was observed in 2 patients and perfusion pattern 1 in another patient. In none of these patients an AL occurred after 90 days of follow-up.

Clinical outcome

A total of 24 time-intensity curves plotted from the ROIs of the anastomosis [afferent ileum or colon and efferent colon in 5 patients ($n = 10$); afferent ileum or colon alone in 14 patients ($n = 14$)] were analyzed (Fig. 5). Of all ($n = 24$) time-intensity curves, 17 (71%) corresponded to perfusion pattern 1, 6 (25%) time-intensity curves to perfusion pattern 2, and 1 (4%) time-intensity curve corresponded to perfusion pattern 3.

AL occurred in 4 (20%) patients. In 1 patient who underwent a right hemicolectomy, the time-intensity curve of the anastomosis on the afferent ileum corresponded to perfusion pattern 3 and the efferent colon to perfusion pattern 1. Postoperatively, this patient developed an acute coagulation disorder with subsequent bowel ischemia and anastomotic leakage as was observed during relaparotomy, after which the patient died. The other 3 patients who developed anastomotic leakage, underwent left-sided resection and the time-intensity curve of the anastomosis on the afferent colon corresponded to perfusion pattern 1. In 1 of these 3 patients, macroscopic ischemia on the afferent colon was observed during relaparotomy.

Table 2. In- and outflow parameters of the quantified time-intensity curves of the ileum and colon.

ILEUM	PATTERN 1 (n=17)	PATTERN 2 (n=8)	PATTERN 3 (n=10)	P-VALUE
Imax, <i>a.u. (range)</i>	131.71 (70.07 – 162.21)	48.75 (13.32 – 64.43)	39.37 (4.15 – 77.85)	<0.001
Ingress slope, <i>a.u./sec (range)</i>	15.45 (4.79 – 17.60)	5.46 (1.55 – 7.41)	1.18 (0.45 – 9.87)	<0.001
Ingress rate, <i>a.u./sec (range)</i>	8.59 (2.49 – 10.17)	1.14 (0.69 – 2.87)	0.16 (0.02 – 0.56)	<0.001
Normalized slope, <i>%/sec (range)</i>	11.99 (8.36 – 14.90)	9.90 (5.75 – 15.22)	4.66 (1.59 – 20.98)	0.018
Tmax, <i>sec (range)</i>	14.50 (12.00 – 25.50)	27.00 (13.00 – 60.00)	215.25 (84.00 – 272.50)	<0.001
Egress slope, <i>a.u./sec (range)</i>	-4.18 (-8.59 – -2.51)	-1.26 (-2.31 – -0.58)	-0.54 (-8.42 – -0.06)	<0.001
AUC 30, <i>% (range)</i>	78.12 (71.96 – 94.51)	95.59 (68.39 – 96.99)	96.46 (49.01 – 97.23)	0.076
AUC 60, <i>% (range)</i>	68.39 (62.21 – 86.28)	90.23 (57.68 – 95.86)	96.84 (49.02 – 96.92)	0.135
AUC 120, <i>% (range)</i>	62.14 (57.53 – 82.08)	82.11 (53.45 – 92.56)	95.91 (49.83 – 96.74)	0.191
AUC 180, <i>% (range)</i>	60.12 (55.38 – 79.87)	77.98 (52.38 – 91.61)	94.07 (94.07 – 94.07)	0.067
COLON	PATTERN 1 (n=95)	PATTERN 2 (n=32)	PATTERN 3 (n=56)	P-VALUE
Imax, <i>a.u. (range)</i>	87.49 (30.83 – 193.32)	46.76 (2.61 – 88.61)	25.22 (2.37 – 86.59)	<0.001
Ingress slope, <i>a.u./sec (range)</i>	9.86 (3.73 – 35.03)	3.41 (0.22 – 11.29)	0.70 (0.11 – 10.98)	<0.001
Ingress rate, <i>a.u./sec (range)</i>	5.51 (1.30 – 21.06)	1.21 (0.12 – 5.12)	0.10 (0.01 – 0.62)	<0.001
Normalized slope, <i>%/sec (range)</i>	12.18 (6.58 – 19.38)	8.16 (3.80 – 18.39)	4.16 (1.43 – 12.68)	<0.001
Tmax, <i>sec (range)</i>	13.00 (8.00 – 39.50)	29.75 (8.00 – 63.00)	231.00 (82.00 – 270.00)	<0.001
Egress slope, <i>a.u./sec (range)</i>	-2.44 (-12.06 – -1.04)	-0.59 (-0.97 – -0.14)	-0.26 (-4.30 – -0.00)	<0.001
AUC 30, <i>% (range)</i>	77.56 (59.59 – 94.85)	94.82 (52.69 – 98.08)	96.91 (78.93 – 99.28)	<0.001
AUC 60, <i>% (range)</i>	68.44 (52.78 – 91.08)	89.52 (42.54 – 96.91)	95.80 (80.53 – 98.11)	<0.001
AUC 120, <i>% (range)</i>	61.85 (48.08 – 95.90)	84.47 (38.40 – 96.70)	93.35 (81.37 – 96.11)	<0.001
AUC 180, <i>% (range)</i>	58.43 (45.96 – 85.49)	81.09 (37.95 – 95.01)	85.59 (81.32 – 93.49)	<0.001

White rows: inflow parameters; Grey rows: outflow parameters; a.u.: arbitrary units; sec: second

Imax: maximum fluorescence intensity, Ingress slope: maximum inflow slope, Ingress rate: mean slope from baseline to maximum fluorescence intensity, Normalized slope: maximum inflow slope in percentage per second, Tmax: time to maximum intensity, Egress slope: maximum outflow slope, AUC30: area under the curve after 30 seconds, AUC60: area under the curve after 60 seconds, AUC120: area under the curve after 120 seconds, AUC180: area under the curve after 180 seconds

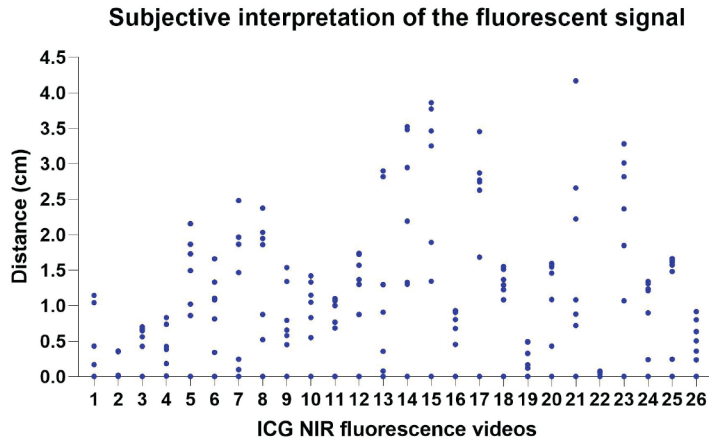


Figure. 2 The mean normalized time-intensity curve with standard deviation of each perfusion pattern for both the ileum and colon.

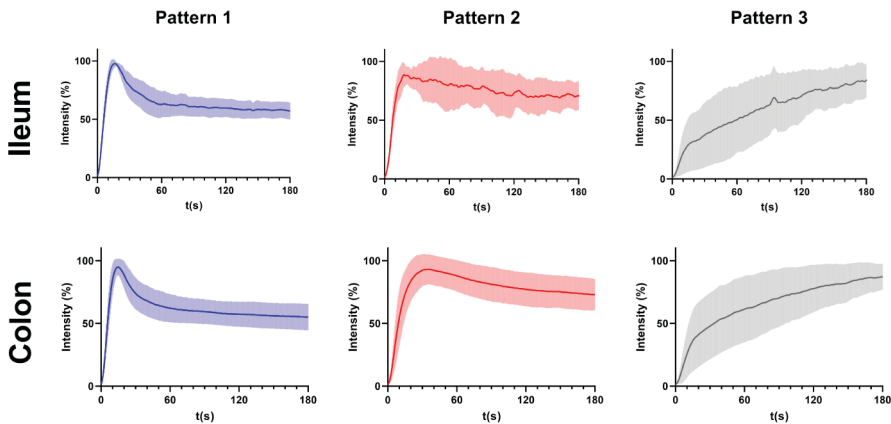


Figure. 3 Inter-observer agreement of the surgeon's subjective interpretation of the fluorescent signal per ICG NIR fluorescence video. Each blue dot represents an intended resection line marked by the surgeon based on the fluorescence signal, with the most proximal marker used as the baseline. An ICG NIR fluorescence video of both the afferent ileum or colon and the efferent colon was analyzed separately. Intraclass correlation (ICC) of 0.378 (95% CI 0.210–0.579).

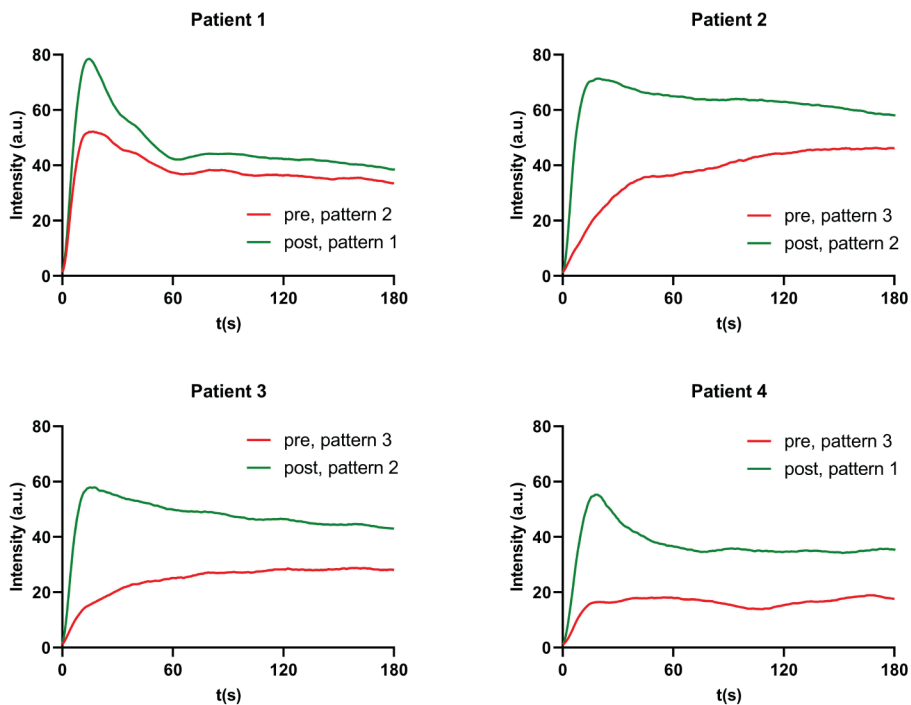


Figure. 4 Time-intensity curves before and after additional bowel resection based on the surgeon's subjective interpretation of the fluorescence signal in 4 patients. The red time-intensity curves represent the fluorescence signal of the intended anastomosis and the green time-intensity curves represent the fluorescence signal of the actual anastomosis after additional bowel resection.

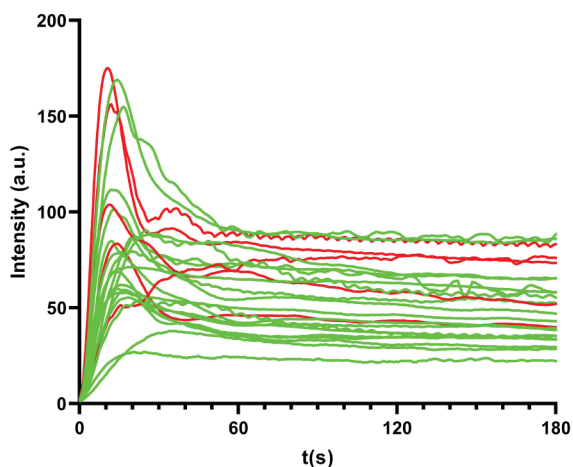


Figure. 5 The absolute time-intensity curves plotted from the ROI of the anastomosis. The red absolute time-intensity curves represents the patients who developed an anastomotic leakage.

Discussion

This prospective dual center cohort study identified quantified bowel perfusion patterns in patients undergoing colorectal surgery by using a standardized imaging protocol. A clear overview of the bowel perfusion was obtained by drawing contiguous ROIs from proximal to distal of the resection line on the ileum and afferent/efferent colon. The quantified time-intensity curves plotted from these ROIs could be divided into three different perfusion patterns. Perfusion pattern 1 implied for well-perfused bowel tissue, as it was mainly observed at the most proximal side of the resection line on the afferent ileum or colon and at the most distal side of the resection line on the efferent colon. In contrast, perfusion pattern 3 implied for poorly perfused bowel tissue, since it was generally present at the avascular region of the ileum or colon from which the vascular branch was already dissected. Perfusion pattern 2 implied for the transition zone, where perfusion pattern 1 transitions to perfusion pattern 3. These three perfusion patterns were identified in each patient and might be a representation of the actual bowel perfusion.

Several cohort studies have investigated quantified bowel perfusion using various quantification methods.^{14–25} In contrast to our study, most of these studies did not use a standardized imaging protocol (i.e., inconsistency in camera-to-target distance, angle of camera on target tissue, type of imaging system and its settings, etc.). Moreover, the ROIs were selected based on the surgeon's subjective interpretation of the fluorescence signal.^{14–16, 18–21, 23–25} As a result, the study results were difficult to compare, which may negatively affect the reproducibility of previously reported quantification methods. Although in our study cut-off values to divide the time-intensity curves among the three perfusion patterns were determined based on qualitative assessment of the quantified time-intensity curves, the subjective factor was limited. Therefore, our quantification method might be more reproducible, which should be validated in larger studies.

Currently, ICG NIR fluorescence bowel perfusion assessment relies on the surgeon's subjective interpretation of the fluorescence signal to guide clinical decision-making, which limits the reproducibility and validity of the technique.^{10–13} This is underlined in this study where a poor-moderate inter-observer agreement of the surgeon's subjective interpretation of the fluorescence signal was observed, with an ICC of 0.378 (95% CI 0.210–0.579).

The ICC was lower compared to the previous published study by Hardy et al.¹² in which a good ICC of 0.753 (95% CI 0.510–0.932) for experts and a moderate ICC of 0.613 (95% CI 0.409–0.856) for non-experts were found. In this study, there were some outliers in the surgeon's subjective interpretation of the fluorescence signal (e.g., ICG NIR fluorescence videos 14, 15, and 21; Fig. 3) for which no clear explanation was found.

A possible explanation for this variability could be the different ways in which surgeons interpret the fluorescence signal, with one surgeon focusing on eventually the most distal fluorescent resection line, another surgeon assessing the fluorescence signal by focusing on the time to maximum fluorescence, and other surgeons being more cautious in defining the resection line based on the fluorescence signal. Although a low ICC is not necessarily detrimental to the clinical outcome (i.e., AL), this study demonstrates the need for quantification of ICG NIR fluorescence imaging to improve the objectivity and accuracy of the bowel perfusion assessment. Especially when bowel length preservation becomes more important, for example in re-resections, Crohn's disease, or in ultralow anterior resection.

The AL rate (20%) in this study was remarkably high when compared to the national AL rate of 6% in 2016 according to the Dutch Colorectal Audit (DCRA).³¹ This AL rate is believed to be an overestimation due to the small sample size as both participating hospitals have annual AL rates that are comparable with the national AL rate by the DCRA. Moreover, the high AL rate could also be explained by the fact that all included patients underwent surgery in tertiary academic hospitals that provide healthcare in highly complex patients in whom the a priori risk of developing AL will be higher. This could also be an explanation of the mortality rate of 10% ($n = 2$) in our study. One patient who developed AL was postoperatively admitted to the intensive care unit for respiratory insufficiency due to an aspiration pneumonia, followed by an acute coagulation disorder which resulted in an acute ischemic limb and bowel ischemia with AL as seen during relaparotomy, after which the patient died. The second patient (ASA-3 with cardiovascular risk factors such as smoking, obesity and diabetes mellitus 2) died of acute myocardial infarction postoperatively. In the other patients with AL, one patient underwent robotic low anterior resection (LAR) and a relaparotomy was performed three days postoperatively to evacuate a hematoma in the small pelvis.

A vital anastomosis was observed during this procedure, however, nine days after primary surgery, the patient developed AL without any signs of ischemia on the afferent colon during relaparotomy. In another patient using long-term prednisolone for IgG4 cholangiopathy, an AL with macroscopic ischemia on the afferent colon was observed. The last patient developed AL in whom LAR was combined with a left nephrectomy. During relaparotomy, a limited AL was observed that required a diverting stoma. Given these highly complex cases, no firm conclusions can be drawn about the high AL and mortality rates found in this study.

Although this pilot study was too small to assess the correlation between the quantified perfusion patterns and AL, the perfusion patterns of the patients who developed AL ($n = 4$) were analyzed. Interestingly, in three of these patients the time-intensity curves of the anastomosis corresponded to perfusion pattern 1. However, in only one of them macroscopic ischemia on the afferent colon was observed during relaparotomy.

This may be explained by the fact that ICG NIR fluorescence bowel perfusion assessment has been implemented as standard care, allowing the surgeon to change the surgical plan intraoperatively based on subjective interpretation of the fluorescence signal. As a result, risk factors other than tissue perfusion might be over-represented in this cohort, since the development of AL is known to have a multifactorial cause. Future studies should investigate the predictive value of each perfusion pattern on the development of AL.

This study has some limitations. First, the primary goal of this exploratory study was to identify quantified bowel perfusion patterns. Therefore, the study design does not allow for any firm conclusions to be drawn about the reliability of the determined cut-off values distributing the time-intensity curves among the three perfusion patterns and the correlation between each perfusion pattern and the development of AL. Thus, there might be a risk of random sampling errors. Additionally, variation in patient-specific hemodynamic factors or the use of vasopressors during the ICG NIR fluorescence measurement could affect the observed perfusion pattern which requires further evaluation because of limited evidence in literature.³² Second, our standardized imaging protocol only allows for extracorporeal video recordings of the ICG NIR fluorescence bowel perfusion assessment. Therefore, in some patients undergoing laparoscopic or robotic left-sided resection, only quantification of the ICG NIR fluorescence imaging video of the afferent colon was possible.

Standardization of the camera-to-tissue distance and angle of the camera-to-tissue can be challenging to maintain during intra-abdominal imaging. However, some studies have shown that quantification of the fluorescence signal using a laparoscopic imaging system might be possible, but the technique of this intracorporeal method is still in its early stages and needs further optimization.^{23, 33}

Lastly, even though the quantification tool is suited to produce proper time-intensity curves in most patients ($n = 18$), the motion tracker of the quantification tool was unable to correct for severe breathing-related movements in two patients. These movements resulted in a fluctuating line in the time-intensity curve, which affected the accuracy of some perfusion parameters (e.g., T_{max} or Egress slope). Although this effect was negligible in our study, the quantification software needs further improvement for daily use.

In the future, larger studies with powered sample sizes should investigate the variation in perfusion patterns and corresponding cut-off values within various bowel parts in correlation to the occurrence of an AL. In addition, these studies should give us a conclusive answer whether quantified perfusion patterns are a reflection of the actual bowel perfusion status and if these patterns could be of added value to predict AL intraoperatively. Moreover, quantification of ICG NIR fluorescence bowel perfusion assessment should be performed intraoperatively to guide the surgeon's clinical decision-making during surgery and to allow immediate modification of the surgical plan when needed.

Conclusion

In conclusion, this prospective cohort study showed that quantification of ICG NIR fluorescence bowel perfusion assessment is a feasible method to differentiate between different perfusion patterns. The use of a standardized imaging protocol could improve the reproducibility of the quantification method. Moreover, the poor-moderate inter-observer agreement of the subjective interpretation of the fluorescence signal between surgeons emphasizes the need for quantification of the fluorescent signal to improve the objectivity and accuracy of the bowel perfusion assessment. Future studies should examine the clinical value of these different perfusion patterns by correlating each perfusion pattern with the development of AL.

References

1. Arron MNN, Greijdanus NG, Ten Broek RPG, Dekker JWT, Van Workum F, Van Goor H, et al. Trends in risk factors of anastomotic leakage after colorectal cancer surgery (2011–2019): A Dutch population-based study. *Colorectal Disease*. 2021 Dec;23(12):3251–61.
2. McDermott FD, Heeney A, Kelly ME, Steele RJ, Carlson GL, Winter DC. Systematic review of preoperative, intraoperative and postoperative risk factors for colorectal anastomotic leaks. *British Journal of Surgery*. 2015 Mar 12;102(5):462–79.
3. Ramphal W, Boeding JRE, Gobardhan PD, Rutten HJT, De Winter LJMB, Crolla RMPH, et al. Oncologic outcome and recurrence rate following anastomotic leakage after curative resection for colorectal cancer. *Surgical Oncology*. 2018 Dec;27(4):730–6.
4. Nachiappan S, Askari A, Currie A, Kennedy RH, Faiz O. Intraoperative assessment of colorectal anastomotic integrity: a systematic review. *Surg Endosc*. 2014 Sep;28(9):2513–30.
5. Karliczek A, Harlaar NJ, Zeebregts CJ, Wiggers T, Baas PC, Van Dam GM. Surgeons lack predictive accuracy for anastomotic leakage in gastrointestinal surgery. *Int J Colorectal Dis*. 2009 May;24(5):569–76.
6. Clifford RE, Fowler H, Manu N, Sutton P, Vimalachandran D. Intra-operative assessment of left-sided colorectal anastomotic integrity: a systematic review of available techniques. *Colorectal Disease*. 2021 Mar;23(3):582–91.
7. Song M, Liu J, Xia D, Yao H, Tian G, Chen X, et al. Assessment of intraoperative use of indocyanine green fluorescence imaging on the incidence of anastomotic leakage after rectal cancer surgery: a PRISMA-compliant systematic review and meta-analysis. *Tech Coloproctol*. 2021 Jan;25(1):49–58.
8. Meijer RPJ, Faber RA, Bijlstra OD, Braak JPBM, Meershoek-Klein Kranenbarg E, Putter H, et al. AVOID; a phase III, randomised controlled trial using indocyanine green for the prevention of anastomotic leakage in colorectal surgery. *BMJ Open*. 2022 Apr;12(4):e051144.
9. Armstrong G, Croft J, Corrigan N, Brown JM, Goh V, Quirke P, et al. IntAct: intra-operative fluorescence angiography to prevent anastomotic leak in rectal cancer surgery: a randomized controlled trial. *Colorectal Dis*. 2018 Aug;20(8):O226–34.
10. Degett TH, Andersen HS, Gögenur I. Indocyanine green fluorescence angiography for intraoperative assessment of gastrointestinal anastomotic perfusion: a systematic review of clinical trials. *Langenbecks Arch Surg*. 2016 Sep;401(6):767–75.
11. Galema HA, Faber RA, Tange FP, Hilling DE, Van Der Vorst JR, De Steur WO, et al. A quantitative assessment of perfusion of the gastric conduit after oesophagectomy using near-infrared fluorescence with indocyanine green. *European Journal of Surgical Oncology*. 2023 May;49(5):990–5.
12. Hardy NP, Dalli J, Khan MF, Andrejevic P, Neary PM, Cahill RA. Inter-user variation in the interpretation of near infrared perfusion imaging using indocyanine green in colorectal surgery. *Surg Endosc*. 2021 Dec;35(12):7074–81.
13. Hardy NP, Joosten JJ, Dalli J, Hompes R, Cahill RA, Van Berge Henegouwen MI. Evaluation of inter-user variability in indocyanine green fluorescence angiography to assess gastric conduit perfusion in esophageal cancer surgery. *Diseases of the Esophagus*. 2022 Nov 15;35(11):doac016.
14. Han SR, Lee CS, Bae JH, Lee HJ, Yoon MR, Al-Sawat A, et al. Quantitative evaluation of colon perfusion after high versus low ligation in rectal surgery by indocyanine green: a pilot study. *Surg Endosc*. 2022 May;36(5):3511–9.
15. Gomez-Rosado JC, Valdes-Hernandez J, Cintas-Catena J, Cano-Matias A, Perez-Sanchez A, Del Rio-Lafuente FJ, et al. Feasibility of quantitative analysis of colonic perfusion using indocyanine green to prevent anastomotic leak in colorectal surgery. *Surg Endosc*. 2022 Feb;36(2):1688–95.
16. D'Urso A, Agnus V, Barberio M, Seeliger B, Marchegiani F, Charles AL, et al. Computer-assisted quantification and visualization of bowel perfusion using fluorescence-based enhanced reality in left-sided colonic resections. *Surg Endosc*. 2021 Aug;35(8):4321–31.
17. Gosvig K, Jensen SS, Qvist N, Nerup N, Agnus V, Diana M, et al. Quantification of ICG fluorescence for the evaluation of intestinal perfusion: comparison between two software-based algorithms for quantification. *Surg Endosc*. 2021 Sep;35(9):5043–50.

18. Ahn H, Son GM, Lee IY, Park S, Kim NS, Baek K. Optimization of indocyanine green angiography for colon perfusion during laparoscopic colorectal surgery. *Colorectal Disease*. 2021 Jul;23(7):1848–59.
19. Amagai H, Miyauchi H, Muto Y, Uesato M, Ohira G, Imanishi S, et al. Clinical utility of transanal indocyanine green near-infrared fluorescence imaging for evaluation of colorectal anastomotic perfusion. *Surg Endosc*. 2020 Dec;34(12):5283–93.
20. Iwamoto H, Matsuda K, Hayami S, Tamura K, Mitani Y, Mizumoto Y, et al. Quantitative Indocyanine Green Fluorescence Imaging Used to Predict Anastomotic Leakage Focused on Rectal Stump During Laparoscopic Anterior Resection. *J Laparoendosc Adv Surg Tech A*. 2020 May;30(5):542–6.
21. Park SH, Park HM, Baek KR, Ahn HM, Lee IY, Son GM. Artificial intelligence based real-time microcirculation analysis system for laparoscopic colorectal surgery. *WJG*. 2020 Nov 28;26(44):6945–62.
22. Seeliger B, Agnus V, Mascagni P, Barberio M, Longo F, Lapergola A, et al. Simultaneous computer-assisted assessment of mucosal and serosal perfusion in a model of segmental colonic ischemia. *Surg Endosc*. 2020 Nov;34(11):4818–27.
23. Hayami S, Matsuda K, Iwamoto H, Ueno M, Kawai M, Hirono S, et al. Visualization and quantification of anastomotic perfusion in colorectal surgery using near-infrared fluorescence. *Tech Coloproctol*. 2019 Oct;23(10):973–80.
24. Son GM, Kwon MS, Kim Y, Kim J, Kim SH, Lee JW. Quantitative analysis of colon perfusion pattern using indocyanine green (ICG) angiography in laparoscopic colorectal surgery. *Surg Endosc*. 2019 May;33(5):1640–9.
25. Wada T, Kawada K, Takahashi R, Yoshitomi M, Hida K, Hasegawa S, et al. ICG fluorescence imaging for quantitative evaluation of colonic perfusion in laparoscopic colorectal surgery. *Surg Endosc*. 2017 Oct;31(10):4184–93.
26. Slooter MD, Mansvelders MSE, Bloemen PR, Gisbertz SS, Bemelman WA, Tanis PJ, et al. Defining indocyanine green fluorescence to assess anastomotic perfusion during gastrointestinal surgery: systematic review. *BJS Open*. 2021 Mar 5;5(2):zraa074.
27. Lütken CD, Achiam MP, Osterkamp J, Svendsen MB, Nerup N. Quantification of fluorescence angiography: Toward a reliable intraoperative assessment of tissue perfusion - A narrative review. *Langenbecks Arch Surg*. 2021 Mar;406(2):251–9.
28. Van Den Hoven P, Tange F, Van Der Valk J, Nerup N, Putter H, Van Rijswijk C, et al. Normalization of Time-Intensity Curves for Quantification of Foot Perfusion Using Near-Infrared Fluorescence Imaging With Indocyanine Green. *J Endovasc Ther*. 2023 Jun;30(3):364–71.
29. Rahbari NN, Weitz J, Hohenberger W, Heald RJ, Moran B, Ulrich A, et al. Definition and grading of anastomotic leakage following anterior resection of the rectum: A proposal by the International Study Group of Rectal Cancer. *Surgery*. 2010 Mar;147(3):339–51.
30. Kulu Y, Ulrich A, Bruckner T, Contin P, Welsch T, Rahbari NN, et al. Validation of the International Study Group of Rectal Cancer definition and severity grading of anastomotic leakage. *Surgery*. 2013 Jun;153(6):753–61.
31. De Neree Tot Babberich MPM, Detering R, Dekker JWT, Elferink MA, Tollenaar RAEM, Wouters MWJM, et al. Achievements in colorectal cancer care during 8 years of auditing in The Netherlands. *European Journal of Surgical Oncology*. 2018 Sep;44(9):1361–70.
32. Al-Taher M, Pruijboom T, Schols RM, Okamoto N, Bouvy ND, Stassen LPS, et al. Influence of intraoperative vasopressor use on indocyanine green fluorescence angiography: first evaluation in an experimental model. *Sci Rep*. 2021 May 6;11(1):9650.
33. Osterkamp J, Strandby R, Nerup N, Svendsen M, Svendsen L, Achiam M. Quantitative fluorescence angiography detects dynamic changes in gastric perfusion. *Surg Endosc*. 2021 Dec;35(12):6786–95.

